UNITED REPUBLIC OF TANZANIA



MINISTRY OF HEALTH COMMUNITY DEVELOPMENT, GENDER, ELDERLY
AND CHILDREN

CONTRACT NUMBER ME/007/MBY/2021- 2022 /G/1 FOR

SUPPLY INSTALLATION, TESTING, COMMISSIONING,
AND TRAINING OF MEDICAL EQUIPMENT
BETWEEN

MBEYA ZONAL REFFERRAL HOSPITAL
AND

KAS MEDICS LIMITED

Form of Contract

THIS AGREEMENT made the 04 day of FEB 20 22 between Mbeya Zonal Referral Hospital, P.O. Box 419 Mbeya, Tanzania (hereinafter called "the PE") of the one part and Kas Medics Limited of Dar es Salaam Tanzania (hereinafter called "the Cupplier") of the other part:

WITEREAS the PE invited Tenders for certain goods and ancillary services, viz., Supply, Installation, Testing, Commissioning and Training Of Medical Equipment (for Njombe RRH) has accepted a Tender by the Supplier for the supply of those goods and services in the sum of 231,292,500/= (two hundred thirty-one million two hundred ninety-two thousand five hundred)Tanzanian shillings, hereinafter called "the Contract Price").

NOW THIS AGREEMENT WITNESSETH AS FOLLOWS:

- 1. In this Agreement words and expressions shall have the same meanings as are respectively assigned to them in the Conditions of Contract referred to.
- 2. The following documents shall be deemed to form and be read and construed as part of this Agreement, In the event of any ambiguity or conflict between the Contract Documents listed below, the order of precedence shall be the order in which the Contract Documents are listed below:-
 - (a) This form of agreement;
 - (b) the Form of Tender and the Price Schedule submitted by the Tenderer;
 - (c) the Schedule of Requirements;
 - (d) the Technical Specifications;
 - (e) the Special Conditions of Contract;
 - (f) the General Conditions of Contract;
 - (g) the Purchaser's Letter of Acceptance; and

3.In consideration of the payments to be made by the PE to the Supplier as hereinafter mentioned, the Supplier hereby covenants with the PE to provide the goods and services and to remedy defects therein in conformity in all respects with the provisions of the Contract

4. The PE hereby covenants to pay the Supplier in consideration of the provision of the goods and services and the remedying of defects therein, the Contract Price or such other sum as may become payable under the provisions of the contract at the times and in the manner prescribed by the contract.

IN WITNESS whereof the parties hereto have caused this Agreement to be executed in accordance with their respective laws the day and year first above written.


FOR PROCURING ENTITY:	FOR LEGAL OFFICER:
Authorized Signature:	Authorized Signal AKILGE MERIKALI
Name: Coolors Marson	Name: Catherine Biffiel 2022
Title: EXECUTIVE DIRECTO	
Date: 04,02, 2022	Date: 4th tolonary 1000
Executive Director Mbeya Zonal Referral Hosp	oital .
FOR THE SUPPLIER: P. O. Box 419 Mbeys - Tanzanis	FOR LEGAL OFFICER:
Authorized Signature:	Authorized Signature:
Name: DOMINUS MBITHT	Name: JARKSON HIGOTYXXXI
Title: Manager CS 170.	Title: ASVOTATE CONTRACT
Date: 04/02/20200 120	Date: 04/02/2028 Morning Company Compa
FOR THE MEDICAL OFFICE WINCHARD	GE (NJOMBE RRH):
Authorized Signature:	WANGILE
Name: WINKEL PHILE	MON KYAMBILE
Title: MEDILAL DEFIC	FR INCHARGE

MEDICAL OFFICER INCHARGE

NJOMBE REGIONAL REFERRAL HOSPITAL
P. O. Box 1044
NJOMBE

O4. Feb. 2022

Date:

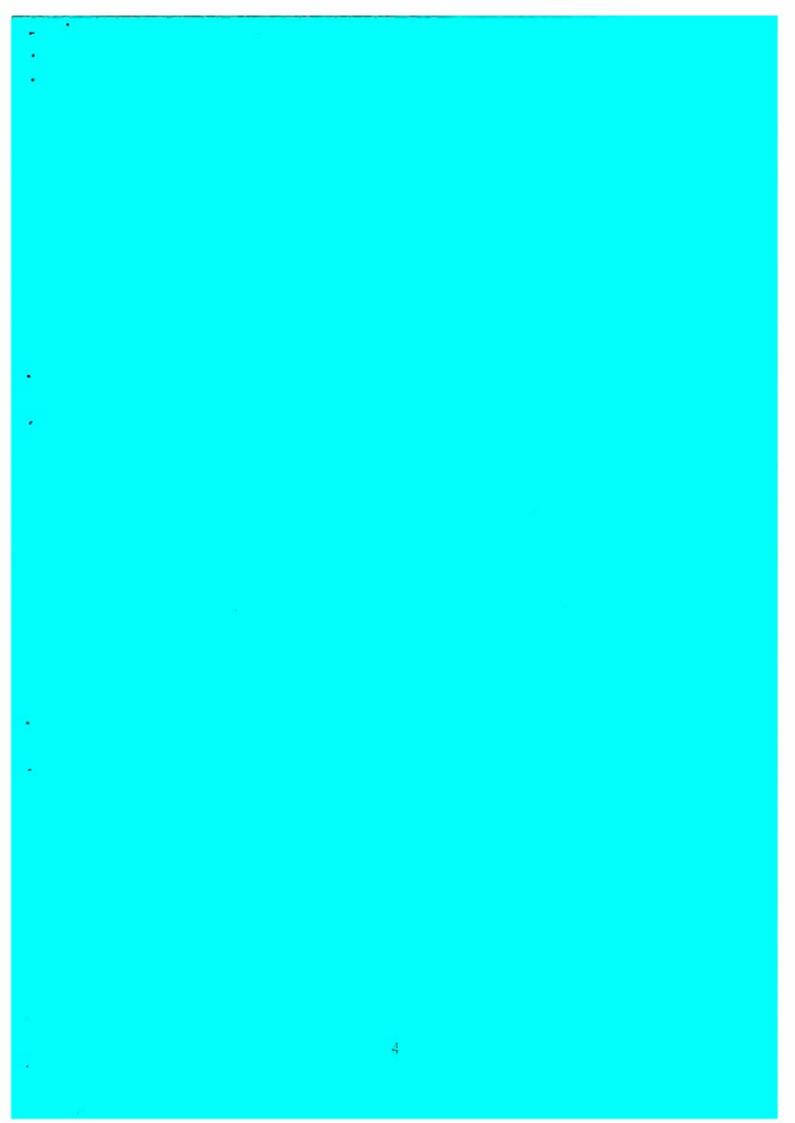

SECTION IV: GENERAL CONDITIONS OF THE CONTRACT

TABLE OF CONTENTS

1. Definitions	
2. Application and interpretation	11
3. Conditions Precedent	
4. Governing Language	12
5. Applicable Law	12
6. Country of Origin	12
7. Standards	
8. Use of Contract Documents and Information; Inspection and	Audit by the Government
of Tanzania	13
9. Patent and Copy Rights	13
10. Performance Security	14
11. Inspections and Test	15
12. Packing	15
13. Delivery and Documents	16
14. Insurance	16
15. Transportation	16
16. Incidental Scrvices	16
17. Spare Parts	17
J8. Warranty	18
19. Payment	18
20. Prices.	19
21. Change Orders	19
22. Contract Amendments	20
23. Assignment	20
24. Subcontracts	20
25. Delays in the Supplier's Performance	20
26. Liquidated Damages	21
27. Termination for Default	21
28. Force Majeure	23
29. Termination for Insolvency	24
30. Termination for Convenience	24
31. Disputes Resolution	
32. Procedure for Disputes	25

33. Replacement of Adjudicator	2!
34. Limitation of Liability	25
35. Notices	2!
36. Taxes and Duties	2!

GENERAL CONDITIONS OF THE CONTRACT (GCC)

1.	Definitions	1.1		e following words and expressions shall have the anings hereby assigned to them:
			a)	The Adjudicator is the person appointed by the appointing authority specified in the Special Conditions of Contract (SCC), to resolve contractual disputes in the first instance, and as provided for in General Conditions of the Contact (GCC) 31 hereunder.
			b)	The Arbitrator is the person appointed by the appointing authority specified in the SCC , to resolve contractual disputes.
			c)	"The Contract" means the agreement entered into between the Procuring Entity (PE) and the Supplier, as recorded in the Contract Form signed by the parties, including all attachments and appendices thereto and all documents incorporated by reference therein.
			d)	The Commencement Date is the date when the Supplier shall commence execution of the contract as specified in the SCC
			e)	"Completion" means the fulfillment of the related services by the Supplier in accordance with the terms and conditions set forth in the contract
			f)	The Contract Price is the price stated in the Letter of Acceptance and thereafter as adjusted in accordance with the provisions of the Contract Days are calendar days
			g	A Defective Goods are those goods which are below standards, requirements or specifications stated by the Contract.
			h)	"Delivery" means the transfer of the goods from the supplier equipment, machinery, and /or other materials which the Supplier is required to supply to the PE under Contract.
			i)	"Effective Contract date" is the date shown in the Certificate of Contract Commencement issued by the Employer upon fulfillment of the conditions precedent stipulated in GCC 3.

	1		
		j)	"The Purchaser" means the person named as purchaser in the SCC and the legal successors in title to this person
		k)	"The Related Services" means those services ancillary to the supply of the Goods, such as transportation and insurance, and any other incidental services, such as installation, commissioning, provision of technical assistance, training, initial maintenance and other such obligations of the Supplier covered under the Contract.
-		1)	"GCC" means the General Conditions of Contract contained in this section.
		m)	The Intended Delivery Date is the date on which it is intended that the Supplier shall effect delivery as specified in the SCC
	1	n)	"SCC" means the Special Conditions of Contract.
	(ပ)	"The PE" means the entity purchasing the Goods and related service, as named in SCC.
	i	p)	"The Supplier" means the individual private or government entity or a combination of the above whose Tender to perform the contract has been accepted by the FE and is named as such in the Contract Agreement, and includes the legal successors or permitted assigns of the supplier and shall be named in the SCC.
	C	q)	"The Project Name" means the name of the project stated in SCC.
	r	7)	"Day" means calendar day.
	S	5)	'Eligible Country" means the countries and territories eligible for participation in procurements financed by the specified institution.
	ť	:)	"End User" means the organization(s) where the goods will be used, as named in the SCC.
	u		"Origin" means the place where the Goods were mined, grown, or produced or from which the Services are supplied. Goods are produced when, through manufacturing, processing, or substantial and major assembly of components, a commercially recognized new produce results that is substantially different in basic characteristics or in purpose or utility from its components.

v) "Force Majeure" means an unforeseeable event which is beyond reasonable control of either Party and which makes a Party's performance of its obligations under the Contract impossible or so impractical as to be considered impossible under the circumstances. For the purposes of this Contract, "Force Majeure" means an event which is beyond the reasonable control of a Party, is not foreseeable, is unavoidable, and its origin is not due to negligence or lack of care on the part of a Party, and which makes a Party's performance of its obligations hereunder impossible or so impractical as reasonably to be considered impossible in the circumstances, and includes, but is not limited to, war, riots, civil disorder, earthquake, fire, explosion, storm, flood, epidemics, or other adverse weather conditions, strikes, lockouts or other industrial action (except where such strikes, lockouts or other industrial action are within the power of the Party invoking Force Majeure to prevent), confiscation or any other action by Government agencies. Specification means the Specification of the Works included in the Contract and any modification or addition made or approved by the Project Manager. W) The Supplier is the person, whether natural or legal

whose Tender to deliver goods or services has been accepted by the Employer

The Supplier's Tender is the completed Tender document submitted by the Supplier to the Employer

10

x)

y)

2.	Application and interpretation	2.1	These General Conditions shall apply to the extent that they are not superseded by provisions of other parts of the Contract.	
		2.2	In interpreting these Conditions of Contract headings and marginal notes are used for convenience only and shall not affect their interpretations unless specifically stated; references to singular include the plural and vice versa; and masculine include the feminine. Words have their ordinary meaning under the language of the Contract unless specifically defined.	
		2.3	The documents forming the Contract shall be interpreted in the following order of priority: (1) Form of Contract, (2) Special Conditions of Contract, (3) General Conditions of Contract, (4) Letter of Acceptance, (5) Specifications (6) Form of tender (7) Any other document listed in the Special Conditions of Contract as forming part of the Contract.	

specified in the SCC; b) Furnishing of Advance Payment Unco-Guarantee. 3.2 If the Condition precedent stipulated on GCC 3.1 is by the date specified in the SCC this contract come into effect; 3.2 If the Employer is satisfied that each of the coprecedent in this contract has been satisfied (exceextent waved by him, but subject to such conditions shall impose in respect of such waiver)he shall prissue to the supplier a certificate of commencement, which shall confirm the start date 4. Governing Language 4.1 The Contract as all correspondence and documents report the contract exchanged by the Supplier and the Playwritten in the language specified in SCC. Subject to GC version of the Contract written in the specified language over its interpretation. 5. Applicable Law 5.1 The contract shall be governed and interpreted in a with the laws of the United Republic of Tanzani otherwise specified in SCC. 6. Country of 6.1 The origin of Goods and Services may be distinct	Conditions 3.1 Precedent	0	Having signed the Contract, it shall come into effect on the date on which the following conditions have been satisfied:-		
Guarantee. 3.2 If the Condition precedent stipulated on GCC 3.1 is by the date specified in the SCC this contract is come into effect; 3.2 If the Employer is satisfied that each of the compression of the Employer is satisfied that each of the compression of the Supplier and the Start date of the Supplier and the Start date of the Supplier and the PE written in the language specified in SCC. Subject to GC version of the Contract written in the specified language specified in SCC. Subject to GC version of the Contract written in the specified language specified in SCC. The contract shall be governed and interpreted in an with the laws of the United Republic of Tanzani otherwise specified in SCC. 6. Country of 6.1 The origin of Goods and Services may be distinct			a) Submission of performance Security in the form specified in the SCC;		
by the date specified in the SCC this contract is come into effect; If the Employer is satisfied that each of the compression of the supplier and the start date. 4. Governing Language 4.1 The Contract as all correspondence and documents in the contract exchanged by the Supplier and the Playmitten in the language specified in SCC. Subject to GC version of the Contract written in the specified language govern its interpretation. 5. Applicable Law 5.1 The contract shall be governed and interpreted in an with the laws of the United Republic of Tanzani otherwise specified in SCC. 6. Country of 6.1 The origin of Goods and Services may be distinct			•		
precedent in this contract has been satisfied (exceextent waved by him, but subject to such conditions shall impose in respect of such waiver)he shall prissue to the supplier a certificate of commencement, which shall confirm the start date. 4. Governing Language 4.1 The Contract as all correspondence and documents in the contract exchanged by the Supplier and the PE written in the language specified in SCC. Subject to GO version of the Contract written in the specified language govern its interpretation. 5. Applicable Law 5.1 The contract shall be governed and interpreted in an with the laws of the United Republic of Tanzani otherwise specified in SCC. 6. Country of 6.1 The origin of Goods and Services may be distinct	3.2	by the date spe	If the Condition precedent stipulated on GCC 3.1 is not met by the date specified in the SCC this contract shall not		
the contract exchanged by the Supplier and the PE written in the language specified in SCC. Subject to GC version of the Contract written in the specified language govern its interpretation. 5. Applicable Law S.1 The contract shall be governed and interpreted in account with the laws of the United Republic of Tanzani otherwise specified in SCC. 6. Country of 6.1 The origin of Goods and Services may be distinct	3.2	precedent in thi extent waved by shall impose in issue to the	s contract has been satisfied (except to the him, but subject to such conditions as he respect of such waiver)he shall promptly supplier a certificate of Contract		
 Law with the laws of the United Republic of Tanzani otherwise specified in SCC. 6. Country of 6.1 The origin of Goods and Services may be distinct 	***	the contract exchange written in the lan version of the Co	nanged by the Supplier and the PE shall be guage specified in SCC. Subject to GCC 3.1. the ontract written in the specified language shall		
	11	aw with the laws of	of the United Republic of Tanzania, unless		
Origin hadonancy of the Supplier.	Country of 6.1 Origin				

7.	Standards	7.1	The Goods supplied under this Contract shall conform to the standards mentioned in the Technical Specifications, and, when no applicable standard is mentioned, to the authoritative standards appropriate to the Goods' country of origin. Such standards shall be the latest issued by the concerned institution.
8.	Use of Contract Documents and Information; Inspection and Audit by the Government of Tanzania	8.1	The Supplier shall not, without the PE's prior written consent, disclose the Contract, or any provision thereof, or any specification, plan, drawing, pattern, sample, or information furnished by or on behalf of the PE in connection therewith, to any person other than a person employed by the Supplier in the performance of the Contract. Disclosure to any such employed person shall be made in confidence and shall extend only as far as may be necessary for purposes of such performance.
		8.2	The Supplier shall not, without the PE's prior written consent, make use of any document or information enumerated in GCC 7.1 except for purposes of performing the Contract.
		8.3	Any document, other than the Contract itself, enumerated in GCC 7.1 shall remain the property of the PE and shall be returned (all copies) to the PE on completion of the Supplier's performance under the Contract if so required by the PE.
		8.4	The Supplier shall permit the Government of the United Republic of Tanzania or / and donor agencies involved in financing the project to inspect the Supplier's accounts and records relating to the performance of the Supplier and to have them audited by auditors appointed by the Government of the United Republic of Tanzania or / and the appropriate donor agencies, if so required by the Government of the United Republic of Tanzania or / and the appropriate donor agencies.
9.	Patent and Copy Rights	9.1	The Supplier shall indemnify the PE against all third-party claims of infringement of patent, trademark, or industrial design rights arising from use of the Goods or any part thereof in the United Republic of Tanzania.
		9.2	The patent right in all drawings, documents, and other materials containing data and information furnished to the PE by the Supplier herein shall remain vested in the supplier, or, if they are furnished to the PE directly, or through the Supplier by any third party, including suppliers of materials, the patent right in such materials shall remain vested in such third party.

10.	Performance Security	10.1	The Performance Security shall be provided to the Employer no later than the date specified in the Letter of Acceptance and shall be issued in an amount and form and by a bank or surety acceptable to the Employer, and denominated in the types and proportions of the currencies in which the Contract Price is payable as specified in the SCC.		
		10.2	The proceeds of the performance security shall be payable to the PE as compensation for any loss resulting from the Supplier's failure to complete its obligations under the Contract.		
		10.3	The performance security shall be in one of the following forms:		
			a) A bank guarantee, an irrevocable letter of credit issued by a reputable bank, or an insurance bond issued by a reputable insurance firm located in the United Republic of Tanzania or abroad, acceptable to the PE, in the form provided in the Tendering Documents or another form acceptable to the PE; or		
(f (a))		+	b) A cashier's or certified check.		
		10.4	The performance security will be discharged by the PE and returned to the Supplier not later than thirty (30) days following the date of completion of the Supplier's performance obligations under the Contract, including any warranty obligations, unless otherwise specified in SCC.		
		10.5	Where circumstances necessitate the amendment of the contract after signature, and such amendment is effected, the PE shall require the Supplier to provide additional Performance Security to cover any cumulative increase of more than ten percent of the initial Contract Price.		

11.	Thomas	999	TI TAT
11.	Inspections and Test	11.1	The PE or its representative shall have the right to inspect and /or to test the Goods to confirm their conformity to the Contract specifications at no extra cost to the PE. SCC and the Technical Specifications shall specify what inspections and tests the PE shall notify the Supplier in writing or in electronic forms that provide record of the content of communication, in a timely manner, of the identity of any representatives retained for these purposes.
		11.2	The inspections and tests may be conducted on the premises of the Supplier or its subcontractor(s), at point of delivery, and/or at the Goods' final destination. If conducted on the premises of the Supplier or its subcontractor(s), all reasonable facilities and assistance, including access to drawings and production data, shall be furnished to the inspectors at no charge to the PE.
		11.3	Should any inspected or tested Goods fail to conform to the Specifications, the PE may reject the Goods, and the Supplier shall replace the rejected Goods to meet specification requirements free of cost to the PE.
		11.4	The PE's right to inspect, test and, where necessary, reject Goods after the Goods' arrival in the PE's country shall in no way be limited or eared by reason of the Goods having previously been inspected, tested, and passed by the PE or its representative prior to the Goods' shipment from the country of origin.
		11.5	Nothing in GCC 10 shall in any way release the supplier from any warranty or other obligations under this Contract.
12.	Packing	12.1	The supplier shall provide such packing of the Goods as is required to prevent their damage or deterioration during transit to their final destination, as indicated in the Contract. The packing shall be sufficient to withstand, without limitation, rough handling during transit and exposure to extreme temperatures, salt and precipitation during transit, and open storage. Packing case size and weights shall take into consideration, where appropriate, the remoteness of the Goods final destination and the absence of heavy handling facilities at all points in transit.
			The packing, marking, and documentation within and outside the packages shall comply strictly with such special requirements as shall be expressly provided for in the Contract, including additional requirements, if any, specified in SCC, and in any subsequent instructions ordered by the PE.

13.	Delivery and Documents	13.1	accordance with the terms specified in the Schedule of Requirements. The details of shipping and or other documents to be furnished by the Supplier as specified in SCC.		
		13.2	For purposes of the Contract, "EXW" "FOB" "FCA", "CIF", "CIP," and other trade terms used to describe the obligations of the parties shall have the meanings assigned to them by the current edition of INCOTERMS published by the International Chamber of Commerce, Paris.		
		13.3	Documents to be submitted by the Supplier are specified in SCC.		
14.	Insurance	14.1	The Goods supplied under the Contract shall be fully insured in a freely convertible currency against loss or damage incidental to manufacture or acquisition, transportation, storage, and delivery in the manner specified in the SCC.		
15.	Transportation	15.1	Where the Supplier is required under Contract to deliver the Goods FOB, transport of the Goods, up to and including the point of putting the Goods on board the vessel at the specified port of loading, shall be arranged and paid for by the Supplier, and the cost thereof shall be included in the Contract Price. Where the Supplier is required under the Contract to deliver the Goods FCA, transport of the Goods and delivery into the custody of the carrier at the place named by the PE or other agreed point shall be arranged and paid for by the Supplier, and the cost thereof shall be included in the Contract Price.		
		15.2	Where the Supplier is required under Contract to deliver the Goods CIF or CIP, transport of the Goods to the port of destination or such other named place of destination in the United Republic of Tanzania, as shall be specified in the Contract, shall be arranged and paid for by the Supplier, and the cost thereof shall be included in the Contract Price.		
		15.3	Where the Supplier is required under the Contract to transport the Goods to a specified place of destination within the United Republic of Tanzania, defined as the Project Site, transport to such place of destination in the United Republic of Tanzania, including insurance and storage, as shall be specified in the Contract, shall be arranged by the Supplier, and related costs shall be included in the Contract Price.		
16.	Incidental Services	16.1	The Supplier may be required to provide any or all of the following services, including additional services, if any, specified in SCC:		
			a) Performance or supervision of on-site assembly and/or		

			start-up of the supplied Goods;
		b)	Furnishing of tools required for assembly and/or maintenance of the supplied Goods;
		c)	Furnishing of a detailed operations and maintenance manual for each appropriate unit of the supplied Goods;
		d)	Performance or supervision or maintenance and/or repair of the supplied Goods, for a period of time agreed by the parties, provided that this service shall not relieve the Supplier of any warranty obligations under this Contract; and
		e)	Training of the PE's personnel, at the Supplier's plant and/or on-site, in assembly, start-up, operation, maintenance, and/or repair of the supplied Goods.
	16.2	inclue upon preva	s charged by the Supplier for incidental services, if not ded in the Contract Price for the Goods, shall be agreed in advance by the parties and shall not exceed the alling rates charged to other parties by the Supplier for ar services.
17. Spare Parts	17.1	any infori	pecified in SCC, the Supplier may be required to provide or all of the following materials, notifications, and mation pertaining to spare parts manufactured or buted by the Supplier:
		a)	Such spare parts as the PE may elect to purchase from the Supplier, provided that this election shall not relieve the Supplier of any warranty obligations under the Contract; and
		b)	In the event of termination of production of the spare parts: i) advance notification to the PE of the pending termination, in sufficient time to permit the PE to procure needed requirements; and
			ii) following such termination, furnishing at no cost to the PE, the blueprints, drawings, and specifications of the spare parts, if requested.

18.	Warranty	18.1	The Supplier warrants that the Goods supplied under the Contract are new, unused, of the most recent or current models and that they incorporate all recent improvements in design and materials unless provided otherwise in the Contract. The Supplier further warrants that all Goods supplied under this Contract shall have no defect, arising from design, materials, or workmanship (except when the design and/or material is required by the PE, specifications) or from any act or omission of the Supplier, that may develop under normal use of the supplied Goods in the conditions prevailing in the United Republic of Tanzania.
		18.2	This warranty shall remain valid for a period specified in the SCC after the Goods, or any portion thereof as the case may be, have been delivered to and accepted at the final destination indicated in the Contract, or for a period specified in the SCC after the date of shipment from the port or place of loading in the source country, whichever period concludes earlier, unless specified otherwise in SCC.
		18.3	The PE shall promptly notify the Supplier in writing or in electronic forms that provide record of the content of communication of any claims arising under this warranty.
		18.4	Upon receipt of such notice, the Supplier shall, within the period specified in SCC and with all reasonable speed, repair or replace the defective Goods or parts thereof, without costs to the PE other than, where applicable, the cost of inland delivery of the repaired or replaced Goods or parts from EXW or the port or place of entry to entry to the final destination.
		18.5	If the Supplier, having been notified, fails to remedy the defect(s) within the period specified in SCC, the PE may proceed to take such remedial action as may be necessary, at the Supplier's risk and expense and without prejudice to any other rights which the PE may have against the Supplier under the Contract.
19.	Payment	19.1	The method and conditions of payment to be made to the Supplier under this Contract shall be specified in SCC.
		19.2	The Supplier's request(s) for payment shall be made to the I'E in writing or in electronic forms that provide record of the content of communication, accompanied by an invoice describing, as appropriate, the Goods delivered and Services performed, and by documents submitted pursuant to GCC 13, and upon fulfillment of other obligations stipulated in the Contract.

		19.3	Payments shall be made promptly by the PE, within sixty (60) days after submission of an invoice or claim by the Supplier. If the PE makes a late payment, the Supplier shall be paid interest on the late payment. Interest shall be calculated from the date by which the payment should have been made up to the date when the late payment is made at the rate as specified in the SCC.	
		19.4	The currency or currencies in which payment is made to the Supplier under this Contract shall be specified in SCC subject to the following general principle: payment will be made in the currency or currencies in which the payment has been requested in the Supplier's Tender.	
		19.5	All payments shall be made in the currency or currencies specified in the SCC pursuant to GCC 19.4	
20.	Prices	20.1	The contract price shall be as specified in the Contract Agreement Subject to any additions and adjustments thereto or deductions there from, as may be made pursuant to the Contract.	
		20.2	Prices charged by the Supplier for Goods delivered and Services performed under the Contract shall not vary from the prices quoted by the Supplier in its Tender, with the exception of any price adjustments authorized in SCC or in the PE's request for Tender validity extension, as the case may be.	
21.	Change Orders	21.1	The PE may at any time, by a written order given to the Supplier pursuant to GCC 22, make changes within the general scope of the Contract in any one or more of the following:	
			a) Drawings, designs, or specifications, where Goods to be furnished under the Contract are to be specifically manufactured for the PE;	
			b) The method of shipment or packing;	
			c) The place of delivery; and/or	
			d) The Services to be provided by the Supplier.	
		21.2	If any such change causes an increase or decrease in the cost of, or the time required for, the Supplier's performance of any provisions under the Contract an equitable adjustment shall be made in the Contract Price or delivery schedule, or both, and the Contract shall accordingly be amended. Any claims by the Supplier for adjustment under this clause must be asserted within thirty (30) days from the date of the Supplier's receipt of the PE's change order.	

		21.3	Prices to be charged by the supplier for any related services that might be needed but which were not included in the Contract shall be agreed upon in advance by the Parties and shall not exceed the prevailing rates charged to other parties by the Supplier for similar services.
22.	Contract Amendments	22.1	Subject to GCC 20, no variation in or modification of the terms of the Contract shall be made except by written amendment signed by the parties.
23.	Assignment	23.1	Neither the PE nor the Supplier shall assign, in whole or in part, obligations under this Contract, except with the prior written consent of the other party.
24.	Subcontracts	24.1	The Supplier shall consult the Procuring Entity in the event of subcontracting under this contract if not already specified in the Tender. Subcontracting shall not alter the Supplier's obligations.
		24.2	Subcontracts must comply with the provision of GCC 5.
25.	Delays in the Supplier's Performance	25.1	Delivery of the Goods and performance of Services shall be made by the Supplier in accordance with the time schedule prescribed by the Procuring Entity in the Schedule of Requirements.
			If at any time during performance of the Contract, the Supplier or its subcontractor(s) should encounter conditions impeding timely delivery of the Goods and performance of Services, the Supplier shall promptly notify the Procuring Entity in writing or in electronic forms that provide record of the content of communication of the fact of the delay, its likely duration and its cause(s). As soon as practicable after receipt of the Supplier's notice, the Procuring Entity shall evaluate the situation and may at its discretion extend the Supplier's time for performance, with or without liquidated damages, in which case the extension shall be ratified by the parties by amendment of Contract.
			Except as provided under GCC 28, a delay by the Supplier in the performance of its delivery obligations shall render the Supplier liable to the imposition of liquidated damages pursuant to GCC 26, unless an extension of time is agreed upon pursuant to GCC 25.2 without the application of liquidated damages.

26.	Liquidated Damages	26.1	of spe pre the pero Good dela ded said	bject to GCC Clause 28, if the Supplier fails to deliver any or all the Goods or to perform the Services within the period(s) cified in the Contract, the Procuring Entity shall, without judice to its other remedies under the Contract, deduct from Contract Price, as liquidated damages, a sum equivalent to the centage specified in SCC of the delivered price of the delayed ods or unperformed Services for each week or part thereof of ay until actual delivery or performance, up to a maximum uction of the performance security specified in SCC. Once the I maximum is reached, the Procuring Entity may consider mination of the Contract pursuant to GCC Clause 26.
27.	Termination for Default	27.1	othe sent	Procuring Entity or the Supplier, without prejudice to any er remedy for breach of Contract, by written notice of default to the concerned party may terminate the Contract if the other y causes a fundamental breach of the Contract.
		27.2	Fun- limi	damental breaches of Contract shall include, but shall not be ted to the following:
			a)	the Supplier fails to deliver any or all of the Goods within the period(s) specified in the Contract, or within any extension thereof granted by the Procuring Entity pursuant to GCC Clause 24; or
			b)	the Supplier fails to perform any other obligation(s) under the Contract;
			c)	Supplier's failure to submit performance security within the time stipulated in the SCC;
		1	d)	the supplier has abandoned or repudiated the contract.
			e)	The Procuring Entity or the Supplier is declared bankrupt or goes into liquidation other than for a reconstruction or amalgamation,
			f)	a payment is not paid by the Procuring Entity to the Supplier after 84 days from the due date for payment;
			g)	the Procuring Entity gives Notice that goods delivered with a defect is a fundamental breach of Contract and the Supplier fails to correct it within a reasonable period of time determined by the Procuring Entity; and
			h)	if the Procuring Entity determines, based on the reasonable evidence, that the Supplier has engaged in corrupt, coercive, collusive, obstructive or fraudulent practices, in competing for or in executing the Contract.
			For th	ne purpose of this clause:

"corrupt practice means the offering, giving receiving or soliciting of anything of value to influence the action of a public officer in the procurement process or contract execution; "coercive practice" means impairing or harming threatening to impair or harm directly or indirectly, any party or the property of the party for the purpose of influencing improperly the action or that party in connection with public procurement or in furtherance of corrupt practice or fraudulent practice; "collusive practices" means impairing or harming, or threatening to impair or harm directly or indirectly, any part or the property of the Party for the purpose of influencing improperly the action or a part or in connection with public procurement or government contracting or in furtherance of a corrupt practice or a Fraudulent Practice "fraudulent practice" means a misrepresentation of facts in order to influence a procurement process or the execution of a contract to the detriment of the Procuring Entity and includes collusive practices among Suppliers, prior to or after submission designed to establish tender prices at artificial non-competitive levels and to deprive the Procuring Entity of the benefits of free and open corapetition; "obstructive practice" means acts intended to materially inspede access to required information in exercising a duty under this Contract; 27.4 In the event the Procuring Entity terminates the Contract in whole or in part, pursuant to GCC Clause 26.1, the Procuring Entity may procure, upon such terms and in such manner as it deems appropriate, Goods or Services similar to those undelivered, and the Supplier shall be liable to the Procuring Entity for any excess costs for such similar Goods or Services. However, the Supplier shall continue performance of the Contract to the extent not terminated.

28.	Force Majeure	28.1	Notwithstanding the provisions of GCC Clauses 25, 26, and 27, neither Party shall have any liability or be deemed to be in breach of the Contract for any delay nor is other failure in performance of its obligations under the Contract, if such delay or failure is a result of an event of Force Majeure.
			For purpose of this clause, "Force Majeure" means an event which is beyond the reasonable control of a Party, is not foreseeable, is unavoidable, and its origin is not due to negligence or lack of care on the part of a Party, and which makes a Party's performance of its obligations hereuncler impossible or so impractical as reasonably to be considered impossible in the circumstances, and includes, but is not limited to, war, riots, civil disorder, earthquake, fire, explosion, storm, flood, epidemics, or other adverse weather conditions, strikes, lockouts or other industrial action (except where such strikes, lockouts or other industrial action are within the power of the Party invoking Force Majeure to prevent
		28.2	If a Party (hereinafter referred to as "the Affected Party") is or will be prevented from performing its substantial obligation under the contract by Force Majeure, it shall give a Notice to the other Party giving full particulars of the event and circumstance of Force Majeure in writing or in electronic forms that provide record of the content of communication of such condition and the cause thereof. Unless otherwise directed by the Procuring Entity in writing or in electronic forms that provide record of the content of communication, the Supplier shall continue to perform its obligations under the Contract as far as is reasonably practical, and shall seek all reasonable alternative means for performance not prevented by the Force Majeure event.

29.	Termination for Insolvency	29 1	The Procuring Entity may at any time terminate the Contract by giving written notice to the Supplier if the Supplier becomes bankrupt or otherwise insolvent. In this event, termination will be without compensation to the Supplier, provided that such termination will not prejudice or affect any right of action or remedy which has accrued or will accrue thereafter to the Procuring Entity.		
30.	Termination for Convenience	30.1	The Procuring Entity, by written notice sent to the Supplier, may terminate the contract, in whole or in part, at any time for its convenience. The notice of termination shall specify that termination is for the Procuring Entity's convenience, the Contract is terminated, and the date upon which such termination becomes effective.		
		30.2	The Goods that are complete and ready for shipment within thirty (30) days after the Supplier's receipt of notice of termination shall be accepted by the Procuring Entity at the Contract terms and price. For the remaining Goods, the Procuring Entity may elect:		
			a)	To have any portion completed and delivered at the Contract terms and prices; and / or	
			b)	To cancel the remainder and pay to the Supplier an agreed amount for partially completed Goods and Services and for materials and parts previously procured by the Supplier.	
31.	Disputes Resolution	31.1	In the event of any dispute arising out of this contract, either party shall issue a notice of dispute to settle the dispute amicably. The parties hereto shall, within twenty eight (28) days from the notice date, use their best efforts to settle the dispute amicably through mutual consultations and negotiation. Any unsolved dispute may be referred by either party to an adjudicator nominated by the appointing Authority specified in SCC.		
		31.2	After the dispute has been referred to the adjudicator, within 30 days, or within such other period as may be proposed by the Parties, the Adjudicator shall give its decision. The rendered decision shall be binding to the Parties.		
		31.3	If eit may arbit SCC	her Party is dissatisfied with the Adjudicator's decision, within days specified in the SCC refer the dispute for ration. If either party within the period mentioned in the has not referred the matter for arbitration the decision become final and binding to the Parties.	

32.	Procedure	32.1	The arbitration shall be conducted in accordance with the			
02.	for Disputes	Jan 1	The state of the s			
	701 Disputes		arbitration procedure published by the Institution named			
		32.2	and in the place shown in the SCC.			
		02,2	The rate of the Adjudicator's fee and administrative costs of			
8			adjudication shall be borne equally by the Parties. The rates			
			and costs shall be in accordance with the rules of the			
			Appointing Authority. In conducting adjudication to its			
			finality each party shall bear its incurred costs and expenses.			
	<u> </u>	32.3	The arbitration shall be conducted in accordance with the			
		34.3				
			arbitration procedure published by the institution named and in the place shown in the SCC.			
33.	Replacement	33.1	Should the Adjudicator resign or die, or should the			
	of		Employer and the Supplier agree that the Adjudicator is not			
	Adjudicator		functioning in accordance with the provisions of the contract,			
	_		a new Adjudicator will be appointed by the Appointing			
			Authority.			
34.	Limitation of	34.1	Except in cases of criminal negligence or willful conduct, and in			
	Liability		the case of infringement pursuant to GCC 8,			
			a) The supplier shall not be liable to the Procuring Entity,			
			whether in contract, tort, or otherwise, for any indirect or			
<u> </u>	1		consequential loss or damage, loss of use, loss of production,			
			or loss of profits or interest costs, provided that this			
			exclusion shall not apply to any obligation of the Supplier to			
			pay liquidated damages to the Procuring Entity; and			
Ē E			b) The aggregate liability of the Supplier to the Procuring			
			Entity, whether under the Contract, in tort or otherwise,			
			shall not exceed the total Contract Price, provided that this limitation shall not apply to the cost of repairing or replacing			
			defective equipment or to any obligation of the Supplier to			
			indemnify the Procuring Entity with respect to patent			
			infringement.			
35.	Notices	35.1	Any notice given by one party to the other pursuant to this			
			Contract shall be sent to the other party in writing or in electronic			
			forms that provide record of the content of communication and			
			confirmed in writing or in electronic forms that provide record of			
	15		the content of communication to the other party's address			
222.33			specified in SCC.			
		35.2	A notice shall be effective when delivered or on the notice's			
36.	Taxes and	36.1	effective date, whichever is later. A foreign Supplier shall be entirely responsible for all taxes, stamp			
50.	Duties	50.1	duties, license fees, and other such levies imposed outside the			
	Duties		United Republic of Tanzania.			
		36.2	If any tax exemptions, reductions, allowances or privileges may be			
			available to the Supplier in the United Republic of Tanzania the			
			Procuring Entity shall use its best efforts to enable the Supplier to			
	\ \		benefit from any such tax savings to the maximum allowable			
			extent.			

36.3	A local Supplier shall be entirely responsible for all taxes, duties,
	license fees, etc., incurred until delivery of the contracted Goods to
	the Procuring Entity.

SECTION V: SPECIAL CONDITIONS OF CONTRACT

Special Conditions of Contract (SCC)

The following Special Conditions of Contract (SCC) shall supplement the GCC. Whenever there is a conflict, the provisions herein shall prevail over those in the GCC. The corresponding clause number of the GCC is indicated in parentheses.

SCC Clause Number	GCC Clause Number	Amendments of, and Supplements to, Clauses in the GCC
	Definitio	ons (GCC 1)
1.	1.1(j)	The Purchaser is: Mbeya Zonal Referral Hospital, P. O. Box 419, Mbeya, Tanzania.
2.	1.1(p)	The Supplier is: KAS MEDICS LIMITED
3.	1.J(q)	The Project is: Tender for supply ,installation ,testing ,commissioning and training of medical equipment
		Contact No. ME/007/MBY/2021- 2022 /G/1
	Governir	ng Language (GCC 4)
4.	4.1	The Governing Language shall be: English
	Applicab	ele Law (GCC 5)
5.	5.1	The Applicable Law shall be: Laws of the United Republic of Tanzania
	Country	of Origin (GCC 6)
6.	6.1	Country of Origin is: N/A
	Performa	nce Security (GCC 10)
7.	10.1	The amount of performance security, as a percentage of the Contract Price, shall be: Ten percent (10%) of the Contract Price in the form of Unconditional Bank Guarantee
8.	10.4	After delivery and acceptance of the Goods, the performance security shall be reduced to two (2) percent of the Contract Price to cover the Supplier's warranty obligations in accordance with GCC 18.2.

	Inspec	ctions and Tests (GCC 11)
9.	11.1	Inspection and tests prior to shipment of Goods and at fina acceptance are as follows:
		Quality and quantity inspection shall be carried out prior to shipment of Goods by the manufacturer(s) at the supplier's own expense and responsibility in terms of the items specified in the specifications. The supplier shall submit the inspection certificate issued by himself which should be attached with the certificate(s) of the manufacturer(s) to the PE in order to ensure that the goods are manufactured in compliance with the contract.
	Packin	g (GCC 12)
10.	12.2	The following SCC shall supplement GCC 12.2:
		The Goods shall be packed properly in accordance with standard export packing specified by the PE in the Technical Specification.
	Deliver	ry and Documents (GCC 13)
11.	13.1	For Goods supplied from abroad:
		Upon shipment, the Supplier shall notify the Purchaser and the Insurance Company by cable the full details of the shipment, including Contract number, description of Goods, quantity, the vessel, the bill of lading number and date, port of loading, date of shipment, port of discharge, etc. The Supplier shall mail the following documents to the Purchaser, with a copy to the Insurance Company:
		(i.) One original plus four copies of the Supplier's invoice showing Goods' description, quantity, unit price, and total amount;
		(ii.) original and four copies of the negotiable, clean, on- board bill of lading marked "freight prepaid" and four copies of nonnegotiable bill of lading;
		(iii.) One original plus four copies of the packing list identifying contents of each package;
		(iv.) Insurance certificate;
		(v.) Manufacturer's or Supplier's warranty certificate;
		(vi.) inspection certificate, issued by the nominated inspection agency, and the Supplier's factory

		inspection report; and
		hispection report, and
		(vii.) certificate of country of origin issued by the chamber of commerce and industry or equivalent authority in the country of origin in duplicate
		The above documents shall be received by the PE at least one week before arrival of the Goods at the port or place of arrival and, if not received, the Supplier will be responsible for any consequent expenses.
12.	13.3	For Goods from within the United Republic of Tanzania:
		Upon delivery of the Goods to the transporter, the Supplier shall notify the PE and mail the following documents to the PE:
		(i.) one original plus four copies of the Supplier's invoice showing Goods' description, quantity, unit price, and total amount;
		(ii.) delivery note, railway receipt, or truck receipt;
_		(iii.) Manufacturer's or Supplier's warranty certificate;
		(iv.) inspection certificate issued by the nominated inspection agency and the Supplier's factory inspection report; and
		(v.) certificate of country of origin issued by the Tanzania Chamber of Commerce, Industry and Agriculture or equivalent authority in the country of origin in duplicate.
3		The above documents shall be received by the PE before arrival of the Goods and, if not received, the Supplier will be responsible for any consequent expenses.
	Insurance	e (GCC 14)
13.	14.1	The Insurance shall be in an amount equal to 110 percent of the CIF or CIP value of the Goods from "warehouse" to "warehouse" on "All Risks" basis, including War Risks and Strikes.
0 0 19 0 19 0 19 0 19 0 19 0 19 0 19 0	Incidenta	l Services (GCC 16)
14.	16.1	Incidental services to be provided are: Not Applicable
	Spare Par	ts (GCC 17)

15.	17.1	Additional spare parts requirements are: Not Applicable
		Supplier shall carry sufficient inventories to assure ex-stock supply of consumable spares for the Goods. Other spare parts and components shall be supplied as promptly as possible, but in any case within six (6) months of placing the order and opening the letter of credit.
	Warranty	(GCC 18)
16.	18.2	In partial modification of the provisions, the warranty period shall be twelve (12) months from date of acceptance of the Goods. The Supplier shall, in addition, comply with the performance and/or consumption guarantees specified under the Contract. If, for reasons attributable to the Supplier, these guarantees are not attained in whole or in part, the Supplier shall, at its discretion, either:
		(a) make such changes, modifications, and/or additions to the Goods or any part thereof as may be necessary in order to attain the contractual guarantees specified in the Contract at its own cost and expense and to carry out further performance tests in accordance with SCC 4,
		or
		(b) pay liquidated damages to the PE with respect to the failure to meet the contractual guarantees. The rate of these liquidated damages shall be 0.20 per cent per day of undelivered materials/goods value up to the sum- equivalent to the amount of ten percent of the contract value.
17.	18.4 & 18.5	The period for correction of defects in the warranty period is: one (1) day from the date of notification received from the purchaser
	Payment	(GCC 19)
18	19.3	Payment for Goods and Services supplied from within the United Republic of Tanzania: Payment for Goods and Services supplied from within the United Republic of Tanzania shall be made in Tanzanian Shillings, as follows:
		(i) Advance Payment: 65% of the contract price after signing the contract
		(ii) On Acceptance: 35 percent of the Contract Price shall be paid to the Supplier within thirty (30) days after the date of the acceptance certificate for the respective delivery issued by the PE.

19.	19.4	Rate to be used for paying the Supplier's interest on the late paymen					
	12.11	made by PE shall be: Not Applicable					
	Prices (GCC 20)						
20.	20.1	Prices shall be adjusted in accordance with provisions in the Attachment to SCC; Not Applicable					
	Liquida	ated Damages (GCC 26)					
21.	26.1	Applicable rate: 0.15% of the contract sum per day of undelivered materials' value.					
		Maximum deduction: is equal to the performance security.					
	Procedure for Dispute Resolution (GCC 32)						
23.	32.3	Arbitration institution shall be Tanzania Institute of Arbitrators					
24.	33 1	Place for carrying out Arbitration. Dar es Salaam, Tanzania Appointing Authority for the Adjudicator: Tanzania Institute of Arbitrators					
	Notices	s (GCC 35)					
26.	35.1	PE's address for notice purposes Executive Director Mbeya Zonal Referral Hospital P.O. Box 419,Mbeya Tanzania					
		Supplier's address for notice purposes: Please indicate					
		Kas Medics Limited,					
		P.O.BOX 7856,					
		Dar Es Salaam.					

THE UNITED REPUBLIC OF TANZANIA

MINISTRY OF HEALTH, COMMUNITY DEVELOPMENT, GENDER, ELDERLY AND CHILDREN

Cable referral hospital

Telephone: 2503456/2503351 Fax: 2503577



MBEYA ZONAL REFERRAL HOSPITAL P.O.BOX 419

MBEYA

Please quite:

Ref. No. MZRH/AD.121/345/02/F.

21th December 2021

Kas Medics Limited,

P.O.BOX 7856.

Dar Es Salaam.

RE: ACCEPTANCE OF TENDER NO. ME/007/MBY/2021-2022/G/1

This is to notify you that your Tender dated 26th November 2021 for execution of the Supply, Installation, Testing, Commissioning and Training Of Medical Equipment Tender No. ME/007/MBY/2021-2022/G/1 for the Contract Price of the equivalent of 182,748,000/= Tanzanian shillings for Iringa RRH, 438,230,000/= Tanzanian shillings for Mbeya RRH, 347,262,000/= Tanzanian shillings For Mbeya ZRH, 231,292,500/= Tanzanian shillings for Njombe RRH, 403,296,000/= Tanzanian shillings for Songea RRH, 388,936,000/= Tsh For Songwe RRH and 450,865,000/= Tanzanian shillings For Sumbawanga RRH, as corrected and modified in accordance with the Instructions to Tenderers is hereby accepted by us.

We hereby confirm Tanzania Institute of Arbitrators to be the Appointing Authority, to appoint the adjudicator in case of any arisen disputes in accordance with ITT 44.1

You are hereby informed that after you have read and return the attached draft Contract the parties to the contract shall sign the vetted contract within fourteen (14) working days.

Your faithfully,

Executive Director
Mbeya Zonal Referral Hospital
P. O. Dox 419
Mbeya - Tanzania

Dr. Mbwanji, G.F

EXECUTIVE DIRECTOR

SECTION VI: SCHEDULE OF REQUIREMENTS

SCHEDULE OF REQUIREMENTS

E	MD-Equipment FOR NJOMBE RRH				
	ITEM DESCRIPTION	UOM	Qnty	UNIT PRICE	Total price
1	ICU beds with CPR Capability	EACH	6	6,547,500	39,285,000
2	Refrigerator with thermometer	EACH	2	4,900,000	9,800,000
3	Heavy duty Stretchers and gurneys (wheeled stretchers)	EACH	15	2,500,000	37,500,000
4_	Vein viewers	EACH	_2	3,500,000	7,000,000
5	Automated external defibrilator	EACH	1	3,395,000	3,395,000
6	Laryngoscope set	EACH	3	1,800,000	5,400,000
7	Emergency curt	EACH	1	1,500,000	1,500,000
	Total				103,880,000

	ICU-Equipment for NJOMBE							
	ITEM DE	UOM	Qnty	U/PRICE	Total Price			
1	ICH Beds with CPR capability	EACH	15	6,547,500	98,212,500			
2	Fluid warmer	LACH	2	4.803,000	9,600,000			
3	Laryngoscope with stylet and boudge	EACH	2	1,800,000	3,600,000			
4	Vein Viewers	EACH	2	3,500,000	7,000,000			
5	Crash Trolley (cart)		6	1,500,000	9,000,000			
	Total				127,412,500			

Total cost of equipments for both ICU and EMD is 231,292,500/= Tanzanian Shillings

DELIVERY PERIOD:

Delivery period for goods in all lots shall be within four (4) months from the date of signing of contract / issuing of purchase order.

SECTION VII: TECHNICAL SPECIFICATIONS

	Equipment Description	Technical specifications	COMPLY/ NOT
1	ICU Beds	Fully Motorized ICU Bed) 5 Section PP Tops, 125mm Twin Wheel Castors. Central Locking Mech., Rubber Buffers at 4 corners Handset, ACP Box, Battery Back Up, SMPS Bed Extension, Linen Holder, Night Lamp. Angle Indicator.Polymer -Moulded Head and Foot Panels (Removable) - Polymer Moulded Split Safety Rails (2 sets) Urine Bag Holder (Single) S.S Heavy Duty I.V. Pole (2 hooks) Premium mattress, single section, 4", with wave shape on both sides, High quality, high density, flame retardant foam and cover fabric having flame	COMPLY
		retardant, antibacterial, antiskid properties Mattress for Bed Extension Should have facility for Invasive and Non-Invasive	
		ventilation Microprocessor Control suitable for Pediatric and Adult ventilation Electromagnetic Compatible Hinged arm holder for holding the circuit Should have built-in touch colour screen TFT display of minimum 10 inches or more for display of waveforms and Monitored value. Five years comprehensive Maintenance inclusive. Should have in-built facility to upgrade with EtcO2	
7		Facility to Measure and Display: Status Indicator for ventilator mode Battery Indication Alarm Setting Automatic compliance and leakage compensation for circuit and ET Tube Should have facility of log book, for events and alarms with date and time	
2	Ventilator	Should have the following settings: Tidal volume (Minimum at least 50ml, Maximum up to 2000ml) Inspiratory Pressure (up to 80cm of water) Respiratory rate 1 to 80 bpm Apnea back up rate CPAP/PEEP Pressure support FiO2	
		Pause Time Pressure and Flow Trigger Inspiratory Flow up to 120bpm Monitoring and Display of the following Parameters: Airway Pressure (Peak and Mean) Tidal Volume (Inspired and Expired) Minute Volume (Inspired and Expired) Respiratory mechanics, Spontaneous Minute Volume Total Frequency, FIO2 dynamic, Intrinsic PEEP, Plateau Pressure, Resistance and Compliance.	
		Use selector Alarm for all measured and monitored parameters, Occlusion Pressure and Pressure Flow and Volume curves. Modes of Ventilation equipped with newer modes of ventilation: Assist Control, Volume Control, Pressure Control SIMV with pressure support (Pressure and Volume	
		control) PEEP Inverse ratio Ventilation Non invasive ventilation - BIPAP, CPAP. Apnea Ventilator, user	

		selectable, volume and pressure control Should have built-in	
		safety alarms for Airway Pressure High and Low, Minute	
	25	volume, High and Low, Power Failure, Low oxygen, High	
		Respiratory Rate, Air Source in-operable. Should have in-built exhalation filter	
		Humidifier: Servo controlled heated Respiratory Humidifier Temperature of delivered Gas on LED display	
		Temperature should be adjustable Jar should be autoclavable Nebulization assembly compatible with ventilator and circuit.	
		Should have interface facility Flow sensor	
		should have life more than 1 year Expiratory Unit- life	
		should be more than 3 years Data storage facility for at least	
		24 hours Internal rechargeable battery at least 30 minutes	
		backup.	
		Supplied complete with compatible UPS and all standard	
		accessories.	<u> </u>
		Power Supply: 220 - 240V, 50Hz	
		Modular & Suitable for Adult/Pediatric/ Patients monitoring	N
		Minimum 15 inches multi colour ΤΕΓ display screen. Five	
	40	years comprehensive Maintenance inclusive.	
		Eight Channel digital and waveforms/traces display.	
		Capability of storage of patient data and printing of patient	
		report.: Facility to monitor and display:-ECG, Respiration, NIBP,	
		SpO2, EtCO2 and	
		Temperature. ECG	
3	Monitor	Multichannel (up to 12 lead) ST segment analysis.	
		3 or 5 lead with cascade waveform facility.	
		Monitoring, Diagnostic & OT modes of monitoring ECG	
		lead Simultaneous Multi - lead ECG monitoring of 7 ECG	
3	5. %	lead. HR range 20-350 bpm. HR/PR Source selection facility from Automatic, SpO2 IBP	
3		and NIBP PULSE OXYMETRY: Display of	
		Plethysmograph with Pulse strength indicator &SpO2 values	8
		and perfusion index.	
		SpO2 range 1 - 100% and PR Range 20 - 230 BPM	
		Electrocardiogram (ECG) digital monitor and recorder, 12-	
		leads detection, multi-channel recording, portable, AC and	
	2 San	battery powered, with printer and accessories. Five years	12
		comprehensive Maintenance inclusive.	
		ECG diagnostic monitor and recorder with printer ECG analysis and full interpretation (rhythm and events), real-	
4	ECG	time and manual.6-channels recording.	
		BCG Features: 12 standard derivations aVR, aVL, aVF, I, II,	
		III, and V1 - V6	
		Simultaneous 12-leads acquisition adjustable ECG	
		acquisition and visualization modes ECG gain 2.5, 5, 10, 20	
		mm/Mv and Auto, accuracy +-5%	
		mm/Mv and Auto, accuracy +-5%	

1	Adjustable ECG sweep (trace speed in mm/s) HR range 30 -	
	300 bpm with rhythm analysis Common Mode Rejection	
	Ratio (CMRR) >89 dB.	
	Frequency response (minimum guaranteed) 0.05 - 159 Hz,	
	accuracy of input signal reproduction +/-5%, calibration	
	signal 1 mV +/- 5% Input Impedance > 2.5 MOhm or >	
	50MOhm.	
	Internal noise level <15 mV (p-p).	
	Leakage current to patient <10 micro A With integrated	
	keyboard, built-in printer with thermal printing head.	
	Built-in rechargeable battery, autonomy >2.5 hours or 800	
	examinations.	
	Automatic switch to battery in case of power failure and	
	automatic recharge on connection to mains.	
	ITEMS SUPPLIED WITH: 1 x patient cable 6 x reusable	
	chest electrodes, suction	
	ball type.	
	4 x reusable clamp electrodes 1 x supply of 960 thermal Z-	
	folded sheets 300ml of ECG conductive gel	±.,
	1 x spare rechargeable battery pack Power Input: 240 VAC,	
	50Hz	1
	Complete with vascular, cardiac and curvelinear probes and	
	Jelly for use in Ambulance and in the Emergency Room.	5
	Five years comprehensive Maintenance inclusive.	+9
	Capable of generating imaging procedures involving lungs,	
	heart, abdomen, polvis, blood vessels, musculoskeletal and	10.00 m
	soft tissue.	
	CONSOLE: Laptop style console design, optional touch	<u> </u>
	screen combined with conventional user control panel	77
	Battery Duration: minimum 2 hours under normal use	
	conditions Supplied complete with clear protective control	
	panel cover for infection control. Imaging Focusing:	
92	Adjustable focal depth, synchronization of focal zone to the	lan di
	selected scanning depth.	
Portable	Zooming Capability with automated image optimization.	
ultrasound	Image Orientation:	
	Capable of lateral and vertical Inversion (in B-mode) Image	
	Modes: 2D Imaging, M-Mode, B/M mode, Dual 2D/Colour	
	Imaging mode with Cine loop.	
	Doppler, Colour Doppler Imaging (CDI), Power Doppler	
	Imaging (PDI), Duplex, Continuous wave Doppler, Triple	3
	mode (optional)	10
	Software Application that include at least:	
	Obstetrics/Gynecology measurements and calculations.	
	including gestational see mean, mean sac diameter, femur	
	length, crown-rump length, bipartetal diameter and	1
No.	abdominal circumference, enabling estimation of gestational	
	age.	
	Vascular/basic cardiac quantification Measurements	

1		capability (distance, area and circumference by ellipse and	
		trace method) Equipment with write-zoom function available	
		Screen annotations capture patient data, date and time,	
		scanning	
		protocols, probes. Monitor and Display: High Definition	
		(HD) digital black and white and colour liquid crystal	
		display (LCD) monitor of at least 25 cm diagonal (across),	
		with reflection filter.	
		Broadband Curvilinear transducer of at least 5-2 MHz and	
		12-5 MHz transducer Power Supply: 220 - 240V, 50 Hz	
		• Portable	2
		• Sample volume 110µl	
		Result in one min after sample aspiration	
6	Blood gas analyzer	Power supply -220v with rechargeable battery at least	
		42mAh	
		At least 10 parameter	
		pH, pO2, pCO2, Na, K, Ca, Cl, Glu, Lac and Hct	
		The machine shall be portable on four wheels and with a	
12		handle for transportation. The suction pump must be totally	
		oil-free diaphragm type.	
		Must have maintenance free pumps of international design	24
		for continuous use Motor shall be of Class "F" insulation to	
		operate in ambient temperature to withstand up to 50oC,	
		with thermal cut-outs Able to produce minimum vacuum of	24
	i	790mm Hg and which must be adjustable and monitored by	(32500 998)
		vacuum gauge of suitable range.	
	- W	The suction capacity must be 25 liters per minute and can be	
1		regulated It must have two bottles of 2l each. Each made of	
	<u> </u>	unbreakable polycarbonate with ABS Lid with float	
7	Suction machine	(overflow control device) The jars must be graduated in cc	
		levels.	
		The suction bottles shall be autoclavable On/Off Switch and	
g 6		power indicator must be available. Shall provide foot switch.	
		Base, top and panel made of rust proof and corrosion	
		resistant moulded ABS.	
		Accessories:	
		Spare bottles: 02nos, Lid: 02nos, Rubber Seals: 02nos,	
	Y .	Blades: 02nos, Suction	
		Tubing set at least 5metres: 02nos,	
		Spare fuse: 01 set and Bacterial filter: 05 nos.	
		Supplied complete with all standard accessories Power	
100	A	Supply: 220 - 240 V, 50Hz	
		Made of aluminium and high density polyethylene	
		5" castors standard with five drawers Drawers made of	
		aluminium composite and high density polyethylene Built-in	
8	Crash Cart trolley	Security Rail Top corrosion resistant, high density	
		polyethylene 5	
		4 qt Sharps Dispenser with mount which can be mounted on	
		left or right along with waste container	

	1	Mount made of high density polyethylene Waste Container	
		with Mount which can be mounted on left or right side along	
		with sharps dispenser	
		Mount made of high density polyethylene	
		Crash Cart Handle: Made of high density polyethylene 360	
		degree Locking Defibrillator Mount with Security Straps:	
		Holds up to 15lbs.	
		Made of high density polyethylene Crash Cart Cardiac	
		Board: Made of high density polyethylene: Made of high	
		density polyethylene Oxygen Tank Mount with Security	
		Straps: Made of high density polyethylene.	
		Holds sizes D & E oxygen tanks Telescoping I.V. Pole with	
		Mount: Two loop design.	
		Extends to a maximum of 72 inches Breakaway Drawer	
		Locks: Individual drawers or gang lock for all drawers	
		available	
	All Views	Features Delivered fully assembled, no tools required Top	
		constructed of solid high density polyethylene 100% Total	
		Replacement Lifetime Guarantee 31 x 42 x 24 inches (width,	
		height depth), 88 pounds Lightweight aluminium composite	87
		construction Multiple accessories available for any	7.79
		application 5" enclosed high compressive nylon rubber	100
10.00	Lane	castors Adjustable and customizable built in track system	
		3 Set for Adults and 2 Sets for Children (Marc and Miller	100
	X 200	Type) Large hollow, cylindrical, slightly ribbed handle.	SIGN NO.
		Handle made of either Chromium plated or	*
		Stainless Steel	
170		Can be opened to insert two batteries (type LR 14, size C.	
9	Laryngoscope set	1.5V) Stud contact, fitting various sizes and types of	
	Lary ngoscope set	depressors With a set of four stainless steel depressors, with	
		halogen bulb Marc. Type Curved Nr 2, length approx.	E.
		110mm Curved Nr 3, length approx. 135 mm Curved Nr 4,	2.
	10	length approx. 155 mm Miller Type Straight Nr 1, length	
	2	approx. 100 mm Supplied with: - 1 x Durable protective	
		plastic box or padded vinyl case - 4 x Spare halogen bulb	
		(one for each depressor) - 2 x Dry cell, alkaline, "C" 1.5V	
		Electrical powered with accessories Portable, compressor	
		driven nebulizer pump Easy to operate and sturdy design for	
		use in demanding environment Cup capacity minimum 3ml	
		to max 10ml Nebulization approximate 0.3 to 0.8 ml/min	
		Residual Volume maximum 2ml Flow delivery range (under	
10	Nebulizer	load) 0.5 t0 max 10 L/min Operating temperature +5 to +50°	
		C Humidity up to 65% Power Supply 220 - 240V, 50Hz,	
	1	50W Supplied with: 1 atomizer body piece 1 pediatric	
		reusable mouth piece 1 adult reusable mouth piece 2 air	1
		tubing 9mm diameter and 1 m length Dosage cup Reusable	
		pediatric and adult masks	
	Pland and fluid	Fluid Temperature Range: 33 - 37°C Heat Transfer Method:	
11	Blood and fluid	Dry heat Time to heat from 23°C to usable range (33 - 37°C)	
	warmer	: 30 - 40 minutes	

	1	High Temperature protection set point: 37°C Temperature:	F .
	1	Operation Mode: +5°C to +40°C Humidity: Operation Mode:	
		-30% to 75% non-condensing Supply Voltage: Warmer, 15	
		VDC Power Supply: 220 - 240V, 50Hz	
		One Channel at least Capable of accepting any kind o fluids	
		(solutions and medications) Pump Capabilities: Flow	
		Range: 0	
	A.	1 to > 999 ml/hr Increments: 0	
		1 - 100 ml/hr Keep Vein Open (KVO) Rate: 1 - 5 ml/hr	-
	41	Volume to be Infused Selector (VTBI): 1 - 9999 ml Flow	
		Rate Accuracy of +/- 5% When multiple channel automatic	
		piggybacking Ingress protection not less than IPX2 Front	
			!
		Panel lockout Self-check carried out on powering on Events	
		Stored System: Log book Pause Infusion Facility required	
		Anti-bolus System to reduce pressure on sudden release of	
		occlusion IV Set Free-Flow Protection and Air Trapping	
		Capability Needleless IV connection "Dose Error" reduction	
		system preferable Drug library software available, including	
		updates (free during warranty)	
		Air Bubble Detector with single and cumulative functions	0.00
		preferable Clearly	
		visible optical alarms Acoustic Alarm not less than 45Db	
		Real Time Display Availability of a Nurse call system	
		connectable to a staff alerting system, 24V/0	3
		2A static or dynamic preferable Continuous operation within	
		specification in ambient temperature of at least 5 - 40oC,	
		Relative humidity of at least 10 - 90% noncondensing	
12	Infusion Pump		
12	mrarion i wiip	Monitored and Displayed Parameters (color and graphic	
		preferable) Flow Pressure Dose Availability of software to	
		monitor the delivery of drugs preferable Alarms Audible	
		alarm required with volume control Momentary silence less	
		than 2 min	
		Occlusion upstream and downstream Air in line and System	
		malfunction Set loaded improperly and Door Open Infusion	
		Complete and Loss of mains power Low Battery and	
		Clinical Advisory Messages Consumables labeled "single	
		use" Compatible Administration Set: 100	
		Compatible Administration Sets micro-bore and macro-bore:	
		100 Compatible long Administration Sets both micro-	
		bore/small and macro-bore or long extension sets: 100	
		Accessories Clamp for mounting pump on IV stand Clamp	
		for external transportation preferable Portability Data port	
		required, at least RS 232 and/or USB interface Long analysis	
		software and updates provided	
		Wireless connectivity	
		Event log required and recording Software to diagnose and	
	¥.	calibrate the equipment with access to calibration settings	
		Power Supply Operates from AC mains power: 220 - 240V,	
	250	50Hz In-built rechargeable battery	
		Battery with operating time at least 4 hours at 25 ml/hr	
		Automatic switch from AC mains power mode to battery	

		1	operating mode and vice versa	
			Total re-charging time not greater than 6 hours	and the state of t
			Microprocessor controlled programmed syringe pump	
L			Programming: Up to 99 steps of speed and time' Time	0
			Resolution: 0 to 999 minutes in 1 minute steps Time	
			Resolution can be selected individually for each program	
			step Accuracy: +- 1% Reproducibility: +/-0.2%Syringes:	
			Glass, plastic. Metal syringes from 5 micro-liter to over	
			150ml Flow Rate Range: Depends on the inner syringe	
L	13		diameter 0.4nl/min with a 5ml syringe to 110ml/min with a	
L			150ml syringe	Alternative Co.
			Maximum Force: 300N reducible by a switch to 80N Motor:	
		Syringe pump	Microprocessor controlled brushless long-life BLDC motor	
L			with Neodymium magnets Transmission: Efficient force	
		7.	transmission by a ball screw with highest mechanical load	
			capacity of 12,000N Pusher Travel: 120mm Pusher Travel	
H			Rate: Minimum: 0	
			08 mm/min Maximum: 80 mm/min Speed Control Range: 0	
L			to 999 Non-volatile Memory: Storage of all settings Power	5 5
		2	Supply: 220 - 240V, 50Hz Interface: RS-485 or RS-232	
		5	automatic valve control Remote Control: 0 - 10V Operation	7 7
		0.00	Temperature: 0 - 40oC Operation Humidity: 0 - 90% RH not	
-			condensing	
			Patient Range: Adult, Pediatrics and Neonatal patients High	336
			Resolution, 2.4" colour display Visual and sound alarms	
			Uses AA size alkaline or rechargeable batteries Digital	
		2.0	SpO2 Range: 0 - 100% Resolution: 1%, Accuracy: 70% to 100% +/-2% Refreshing Rate: < 13 seconds Pitch Tone: Yes	
		Portable Hand held	Pulse Rate Range: 25 - 250 bpm Resolution: 1 bpm.	South Control
	14	Pulse oximeter	Accuracy: +-2% or +/-1 bpm Refreshing Rate: < 13 seconds	
		T tilbe oximeter	Display: Type: 2.4" color display 320 x 240 pixels	
			Parameter Digital SpO2, Pulse Rate, Pleth bar and SpO2	
		5 1	waveform	
			Alarm Audible alarm, audible button tone Supports Pitch	
			Tone and multi-level volume	
			General Description Modular and Suitable for	
		14	Adult/Paediatric/ Patient monitoring Minimum 15" multi-	
			colour TET display screen Eight Channel digital and	
			waveforms/traces display Capability of storage of patient	
			data and printing of patient reports. Five years	
		Central Monitoring	comprehensive Maintenance inclusive.	4 4
	15	Station 8 Channel	Parameters: Eight digital and waveforms/traces display	
		Station o Chamics	Facilities to monitor and display ECG, Respiration, NIBP, Et	
			CO2, SpO2 and Temperature ECG Multichannel (uo to 12	
			lead) ST segment analysis 3 or 5 lead with cascade	
		5	waveform facility Monitoring, Diagnostic and OT modes of	
			monitoring of ECG Simultaneous Multi-lead ECG	i
			monitoring of 7 ECG lead	

		r	
	Heart Rate (HR) Range: 2 - 350 bpm HR/PR Source		
	selection facility from Automatic, SpO2 IBP and NIBP		
	Automatic arrhythmia detection alarm for standard and lethal		
	arrhythmia Pulse OximetryNellcor or Masimo technology		
	Display of Plethysmograph with Pulse Strength indicator and		
	SpO2 values and perfusion index Sp02 Range: 1 - 100% PR		
	Range: 20 to 230bpm ETCO2 Should be Main stream		
	capnography with display of CO2 and digital Values of		
	EtCO2, FiCO2 and RR		
	EtCO2 Range: 0 - 99 mmHg FiCO2 Range 0 - 20 mmHg		
	Flow Rate: 50ml/min NIBP Measurement and display of		
	systolic, diastolic and mean pressure values of NIBP		
	measurement for Adult, Child and Neonate		
	Use selectable alarm settings: Mode: Manual, STAT		
	(continuous 5 minute operation) and automatic (selectable		
	time interval 2 - 90 minutes) Range: 20 - 250 mmHg		
	Temperature Two channel and with two units (oC and o F)		
	selectable Temperature Range: 0 - 50oC		
	Option for differential temperature		
	Should be provided Respiration: RR range 1 - 150 bpm		
	Apnea alarms should be provided Trends and Alarms 72		
	hours		
	Nonvolatile graphical/ tabular trends with zoom facility and		
	separate dedicated trend for storing minimum200 NIBP		
	readings Should have Alarm recall facility for last 24 Alarm		
	events with date, time and message		
	Should have facility to print Graphical trend, tabular trend		
	and alarm recall		
	Recorder In-built dual channel thermal array recorder		
	Include Laser Printer and dual channel strip chart recorder		
	Others Defibrillator and Cautery protection should be		
	provided		
3	•		
	Should work on Mains as well as Battery (backup for 2		
	hours) Automatic zoom in facility in the monitor display		
	Should have facility to download trend data on USB and SD		
	Card Supplied complete with all standard accessories and		
	consumables that will enable the machine to operate		
	Power Supply: 220 - 240V,50 Hz		
	CENTRAL STATION Central Station should have facility		
	to display up to 20 real time waves at a time and upgradable		
	Central Station should have separate patient window for		
	viewing detailed real-time or stored data for individual		
	patient		
	It should have 24 hr stored patient data monitoring trends	100 17 17	
	and 24 hr event review facility		
	The Central Nurse Station should also have the following: -		
	Multi-lead arrhythmia and ST review facility - 50 alarms		
	strips storage per bed - Offer wave review with 24 hr full		
	disclosure - Optional facility for dual display for detailed		
	analysis of individual bed without compromising on full ICU		
	monitoring		

Facility for interfacing Holter data for analysis, in case of	İ
the Holter from the same brand is available	
Export the ICU Patient data to Holter for analysis	
Remote display (Slave) facility should be available	
Real time recording thru Dual Channel Recorder	
Facility for interfacing a laser printer for printing patient	
information and trend formats	
Advanced arrthythmia analysis package of at least 20	
arrthythmia analysis	
12 lead ECG Monitoring and view possible at Central Nurse Station	
Continuous full disclosure of up to 4 configurable waves per	
patient	
Operate on Microsoft Windows NT workstation operating system	
Supplied with 19" Flat Screen TFT display, Laser Printer and Recorder, UPS	
- The entire networking and cabling witrh hardware Wall mounts	
Power Supply: 220 - 240 V, 50Hz	
Should be a Low Energy Biphasic defibrillator monitor with	
Recorder, having capability to deliver shocks from 2 Joules	10 10 14
to 200Joules. Five years comprehensive Maintenance	100
inclusive.	
Should monitor ECG through paddles, pads and monitoring	
electrodes and defibrillate through pads and paddles	Ħ
Should compensate for body impedance for a range of 25 to	
150 ohms.	
Should have charging time of less than 5 seconds for	
maximum energy.	
Should have High resolution more than 8-inch color display	
for viewing monitoring parameters like ECG, SpO2, NIBP	50
and EtCO2 with 4 waveform capability of 4 seconds	
Both Adult and Pediatric paddles should be available Should	25.0
have event summary facility for recording and printing at	
least 55 events	
Should have a battery capable of usage for at least 5 hours of monitoring	
Should be capable of printing Reports on event summary,	
configuration, self-test, battery capacity etc. Should have	
facility for self-test/cheek before usage and set up function.	
Should have facility to monitor parameters like SpO2, NIBP	
and etCO2 along with non-invasive pacing (Demand and	
Fixed mode) facility	
Should be able to upgrade the defibrillator for 12 lead ECG	
monitoring and ECG transmission System	
Configuration Accessories, spares and consumables:	
Defibrillator with AED and external Pacemaker - 1pc Adult	
with built in Pediatric	
• (2)	1

16 Defibrillator

Adult SpO2 reusable Sensor -	Cables - 1pc ECG Rolls 50
Hose - 1pc EtCO2	
Tubing (box of 20) -1box AEI Adults - 10 pairs with Each un	it.
The unit shall be capable of o	perating continuously in
ambient temperature of 5 to 45 up to 95%	oc and relative humidity of
Shall meet General Requireme	nts of safety for
Electromagnetic Compatibility Power Input: 240 VAC, 50Hz	
Illumination: Pressurized halog	gen Jamn Imaga Pagalutian
1280 x 1024 pixels Connection	Interface: USR 2.0 with 3m
cable System Requirements: W	Vindows XP Service Pack
Wall mounted Electrical Rating: Lamp 3.5V I	DC, 810mA USB: 5V DC
150mA Focal length:114mm as	nd Magnification:2.2X
Constructed from ABS and Act	rylic Plastic or Stainless Steel
Automatic Image Brightness ar	nd white balancing for optimal
ımage	
quality Supplied complete with	
Range of lenses not smaller that	n -20D to +29D with steps
not greater than ID. Anti-reflect	ion lens Magnification: 12 -
15X Apertures: Small, Large ar	d Semi Circle, Fixation Star
Colour Temperature: Cool Whi	te in the range 3100 - 5500K
Wall mounted Light Intensity: 8,000 - 12,000 and aspherical optical system R	lux. Dust free sealed optics
and depretation option by stem to	ed-free, Blue, Green and
Opthalmoscope polarization filters Handle with lens: Glass or Plastic Batteries:	AA or rachamarkia D.
life at least 5 hours of use on ful	Il charge or fresh betteries
Accessories: Battery Charger (a	s applicable to rechargeable
type only) Sufficient light bulbs	for 3 years use
Rechargeable Battery 1.5V.	is a years ase.
Stainless steel shelves and railin	gs Available in full stainless
steel/powder coated frame. Stair	aless steel bottom and top
Instrument trolley shelves with railing on top shelf	Frame Mounted on 100 mm
diameter wheels Overall Size: L	710 mm x W460 mm x
H830 mm	
Adjustable Mayo Adjustable Mayo	
table freight adjustable by foot 75 mm	n swivel castors Dimensions:
Width 60 cm, Depth 40 cm and 1	Control of the contro
• Dimensions(mm): 850x500x39	mm
• Film: 14 x 17"	
• View area: 730x442mm	
21 x-ray viewer Lamp: CCFL 12pcs Luminance: 12.000lux or more	
21 x-ray viewer • Luminance: 12,000lux or more • Power consumption: 60W	
Power: 220VAC 50/60HZ	
• Life Time: over 80,000hr	
• Film Clipping: Spring Roller or	similar

Digital Mobile Xray

22

This Machine should be able to provide a minimum of 300 images per day. Should have a high frequency generator of 50-150KW, Automatic exposure device, Anatomical programming radiography, overloading protection feature, digital display of KV and mAs. X-Ray tube should be Floor stand mounted.

Axis should rotate 360 degree

Five years comprehensive Maintenance inclusive. High speed rotating anode and exposure should be 50 – 150KV and 0-600mA. Heat strength capacity of the anode at least 150,000HU.

The digital detector (Two fixed Detectors) should be flat panel of latest technology.

The digital workstation should have high speed processors, preview time of 5s or less.

The workstation should provide basic functions for image processing and be compatible to other HIS

Displayed Parameters: The console monitor should display patient ID, Exposure factors, warning sign and other important parameters.

Components: Patient table: Mounted on heavy duty four castors with brakes to allow Longitudinal and lateral movement and better patient position. Floating table with up and down movement Table Size from 1800x800mm to 2200x800mm Patient weight: at least 150Kg Bucky wall stand: Height: 1900mm

Center Height Stroke Range from 400mm to 1600mm Source to image detector should include the range of 90cm to 125cm

Detectors:

Fixed Flat Panel Detectors

Active Image Size at least 17inch x 17inch or 43cm x 43cm Pixel Size at least 140 micron

Dimension: 460 x 460 x 15mm

Dust cover for control unit to be supplied. Protection against insect and rodent ingress to be incorporated.

Electrical Requirements: Should meet Tanzania Electrical Standards (Voltage of between 220-240V with the standard frequency of 50Hz) with type G adaptor System.

Accessories: Multi-tray printer for different X-Ray film sizes (10 x 12, 14 x 14, 14 x 17, 10 x 8). Protective gear (lead apron minimum of 2 small, 2 medium and 2 large), Googles (Minimum 1 small, 1 medium and 1 large). Gonad shield (minimum 2 small, 2 mediums, 2 large), neck collar shield (minimum of 1 small, 1 medium, 1 large), Gloves (Minimum 2 small, 2 medium and 2 large). Radiation hazards warning signs to be supplied with the machine. It should come with the Power Backup System with capacity of power storage for not less than 15 Minutes.

Radiation protective gears: X-ray should come with;(i) two (2) pairs of lead aprons with back protection 0.35/0.25mmPb, (ii) two (2) pairs of Thyroid Shield Model Classic 0.35mmPb (iii) two (2) pairs of Patient Apron with belt 0.50mmPb Leadlite W/G-30 L-30 Printer

Multi-tray printer for different X-Ray film sizes (10 x 12, 14 x 14, 14 x 17, 10 x 8).

Training, Installation and Utilization

Requirements for commissioning: Manufacturer/supplier should perform installation, safety and operation checks before handover. Acceptance tests to be specified and local clinical and technical staff to verify proper and full functioning of device.

Training of user/s: Application specialist shall provide training of users in operation and basic maintenance. Warranty and Maintenance:

Five years comprehensive maintenance should include service, spare parts and labour starting from the day of the acceptance testing of the machine.

Lifetime support; spare parts, consumables should be available throughout the lifetime period of the machine.

Uptake time should be a minimum of 90%.

Proof of locally available technical support personnel, including CVs and work permit for foreign personnel. Availability of technical personnel within the country should be stated; this should include CVs, work permits for foreign personnel.

Software should be flexible and provide the room for upgrade to add new parameters to be measured by the Machine and report format.

Documentation: Operating and service manuals (In English) including lists of important spares and accessories - with their part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community.

Life span: Life span of the machine should be not less than 10 Years.

Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices.

Regulatory Approval / Certification: TAEC, TBS and TFDA

The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assistcontrol Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as 1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFΓ medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressure volume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VΓ, VTspont, MV and MVleak. The volume monitoring should have NTPD to BTPS correction. Monitoring of ie, Frequency and Spont, Frequency Settings range: Trigger Flow/volume, leak adapted PIP 8 to 80cm of water PEEP/CPAP 0 to 25 mbar. Five years comprehensive Maintenance inclusive.

Neonatal ventilator

23

I:E ratio 1:0 to 1:10 Inspired Time 0.1 to 2 sec Expired Time 0.2 to 30 sec Frequency Up to 200 BPM Base Flow (VIVE) 1 to 30 LPM Synchronization Patient synchronization Integrated blender for Oxygen 21 % to 100% Integrated nebulization facility Integrated screen for display of Pressure-Time, Flow-Time and Volume-Time curves Integrated monitoring of FiO2 Monitoring of flow: At the Y piece with facility to activate it Audiovisual alarms with advisory on-screen message: MV high/low, Apnea, tube obstruction, FiO2, high/low high PIP, low PEEP/CPAP, fail to cycle, gas supply low, power failure, ventilator inoperative, alarm log book. The ventilator should have automatic compensation for leakage and should monitor and display leakages The ventilator should show trends of important parameters viz. C,R, FiO2, MAP, etc for evaluation of patient improvement Power Supply: 220 -240V, 50Hz, SCOPE OF

SUPPLY Ventilator on trolley with wheels and brake facility Integrated medical air compressor Humidifier with autoclavable chamber and complete with patient Circuit support arm Nebulization accessories (2 sets)

		Bacterial filters 50 sets Flow sensors 20 sets Oxygen cell and Oxygen connecting hose Air connecting hose Battery back-up (at least 30 minutes)	**
24	Hemoglobinometer	Parameter: Hemoglobin, HCT(Hematocrit) Principle: Optical reflectance · Sample: Capillary or venous whole blood (13-15ul) · Strip: H12 Hemoglobin Test Strip · Speed: ≤ 10 seconds · Measuring Range: 4.0g/dL-25.6g/dL(g/L optional) · Memory: 1200 test results · Automatization: Self-checking, auto-judging and displaying malfunction · Power: DC 6V(Two CR2032 Batteries) · Precision: CV<5%,testing samples including high, medium & low	
25	EMD Beds	Fully Motorized ICU Bed) 5 Section PP Tops, 125mm Twin Wheel Castors. Central Locking Mech., Rubber Buffers at 4 corners Handset, ACP Box, Battery Back Up, SMPS Bed Extension, Linen Holder, Night Lamp, Angle Indicator.PolymerMoulded Head and Foot Panels (Removable) - Polymer Moulded Split Safety Rails (2 sets) Urine Bag Holder (Single) S.S Heavy Duty I.V. Pole (2 hooks) Premium mattress, single section, 4", with wave shape on both sides, High quality, high density, flame retardant foam and cover fabric having flame	
		retardant, antibacterial, antiskid properties Mattress-for Bed Extension	
26	Nasal Cannula (prongs)	Nasal cannula (nasal prongs), device designed for easy administration of oxygen into the patient nose through two small prongs placed in the nostrils. It consists of soft twin prongs nasal tips to ensure equal oxygen flow to both. Adjustable, smoothly finished nasal tips for maximum patient comfort Star lumen main tube to avoid accidental blockage. Made from soft and kink	
27	Wall mounted otoscope	resistant polyvinyl chloride (PVC) material For Adult and Child use Illumination: Pressurized halogen lamp Image Resolution: 1280 x 1024 pixels Connection/Interface: USB 2.0 with 3m cable System Requirements: Windows XP Service Pack Electrical Rating: Lamp 3.5V DC, 810mA USB: 5V DC, 150mA Focal length:114mm and Magnification:2.2X Constructed from ABS and Acrylic Plastic or Stainless Steel Automatic Image Brightness and white balancing for optimal image	
28	wall mounted	Range of lenses not smaller than -20D to +29D with steps not greater than1D. Anti-reflection lens Magnification: 12 - 15X Apertures: Small, Large and Semi Circle, Fixation Star Colour Temperature: Cool White in the range 3100 - 5500K Light Intensity: 8,000 - 12,000 lux. Dust free sealed optics and aspherical optical system Red-free, Blue, Green and polarization filters Handle with On/Off switch. Scratchproof lens: Glass or Plastic Batteries: AA or rechargeable. Battery life at least 5 hours of use on full charge or fresh batteries Accessories: Battery Charger (as applicable to rechargeable type only) Sufficient light bulbs for 3 years use. Rechargeable Battery 1.5V.	

Stainless steel Shelvins and railings Available in full stainless steel/powder coated frame. Stainless steel bottom and top shelves with railing on top shelf Frame Mounted on 100 mm diameter wheels Overall Size: L730 mm x W460 mm x H830 mm Made of stainless steel with removable top tray Height adjustable by foot 75 mm swivel castors Dimensions: Width 60 cm, Depth 40 cm and Height 120 -130 cm Uptake time should be a minimum of 90%. Proof of locally available technical support personnel, including CVs and work permit for foreign personnel. Availability of technical personnel within the country should be stated; this should include CVs, work permits for foreign personnel. Software should be flexible and provide the room for upgrade to add new parameters to be measured by the Machine and report format. Documentation: Operating and service manuals (in English) including lists of Important spares and accessories - with their part numbers and list of equipment and procedures for disposal and any probable hazards to the environment end/or community. Uffe span tiffe span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices Regulatory Approval/ Certification: TAEC, TBS and TEDA The Ventitator should be microprocessor controlled designed for neonatal use. There should be possibility to uggrade with additional features Continuous flow, pressure limited, time cycled ventilator should have following modes available in the unit INM/INPV CPAP including non-invasive vantilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation Apnea back-up ventilation Should have integrated injah resolution TFT medical grade screen (size 4") for roal time display Scalar (Pressure, Flow and Volume against time), and loop (Pressurevolume, volume flow and pressure, flow) pulmonary graphics Digital display of 102, Peak pressure, flowy and pressure monitoring compliance, resistance, lung distention coefficient, (C20C), lung time consta	1	1	Stainless stand chalung and millings Auditable in full stainless	12
shelves with railing on top shelf Frame Mounted on 100 mm diameter wheels Overall Size: L 710 mm x W460 mm x H830 mm Made of stainless steel with removable top tray Height adjustable by foot 75 mm swivel castors Dimensions: Width 60 cm, Depth 40 cm and Height 120 - 130 cm Uptake time should be a minimum of 90%. Proof of locally available technical support personnel, including CVs and work permit for foreign personnel. Availability of technical personnel within the country should be stated; this should include CVs, work permits for foreign personnel. Software should be effexible and provide the room for upgrade to add new parameters to be measured by the Machine and report format. Documentation: Operating and service manuals (in English) including lists of important spares and accessories - with their part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: Life span of the machine should be not less than 10 Years Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Reguletory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMM/PDV CPAP including non-invasive ventilation SIMY, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation with ability to deliver and monitor tidal volume, as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation of pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure monitor in the requency,		A Company		
Made of stainless steel with removable top tray Height adjustable by Foot 75 mm swivel castors Dimensions: Width 60 cm, Depth 40 cm and Height 120 - 130 cm Uptake time should be a minimum of 90%. Proof of locally available technical support personnel, including CVs and work permit for foreign personnel. Availability of technical personnel within the country should be stated; this should include CVs, work permits for foreign personnel. Software should be flexible and provide the room for upgrade to add new parameters to be measured by the Machine and report format. Documentation: Operating and service manuals (in English) including lists of important spares and accessories - with their part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TEDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be microprocessor controlled designed for neonatal use. There should be microprocessor controlled designed for neonatal use. There should be microprocessor controlled designed for neonatal in the unit tMy/IPPV CPAP Jacudding non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation Appea back-up ventilation Should have integrated in high resolution IFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FioQ, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tiidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung d	29			
Made of stainless steel with removable top tray Helight adjustable by foot 75 mm swwel castors Dimensions: Width 50 cm, Depth 40 cm and Helight 120 - 130 cm Uptake time should be a minimum of 90%. Proof of locally available technical support personnel, including CVs and work permit for foreign personnel. Availability of technical personnel within the country should be stated; this should include CVs, work permits for foreign personnel. Software should be flexible and provide the room for upgrade to add new parameters to be measured by the Machine and report format. Documentation: Operating and service manuals (In English) including lists of important spares and accessories - with their part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span; tife span of the machine should be not less than 10 Years. Risk Classification: As per ISO J4971:2007- Application of risk management to medical devices. Reguldary Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilation ISIMY, SIPPY/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure-flow) pulmonary graphirs. Digital display of Flo2, Peak pressure-mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minicute volume, total frequency, sopnataneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built in logbook for recording events like various alarms.		Instrument trolley		
Height adjustable by foot 75 mm swivel castors Dimensions: Width 60 cm, Depth 40 cm and Height 120 - 130 cm Uptake time should be a minimum of 90%. Proof of locally available technical support personnel, including CVs and work permit for foreign personnel. Availability of technical personnel within the country should be stated; this should include CVs, work permits for foreign personnel. Software should be flexible and provide the room for upgrade to add new parameters to be measured by the Machine and report format. Documentation: Operating and service manuals (In English) including lists of important spares and accessories - with their part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As por ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SiNV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low sat1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have inlegrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, How and Volume agaginst time) and loop (Pressurevolume, volume flow and pressure mean airway pressure, cornorl Volume constant, Rate volume ratio etc. Should have built in logbook for recording events like various alarms, integrated monitoring, Integrated volume and press		instrument troney	The state of the s	
Uptake time should be a minimum of 90%. Proof of locally available technical support personnel, including CVs and work permit for foreign personnel. Availability of technical personnel within the country should be stated; this should include CVs, work permits for foreign personnel. Software should be flexible and provide the room for upgrade to add new parameters to be measured by the Machine and report format. Documentation: Operating and service manuals (in English) including lists of important spares and accessories - with their part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilation design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (see 4°) for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (see 4°) for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure mean airway pressure, CPAP/PEEP, Epigratory tidal volume, expiratory minute volume, totae constant, Rate volume ratio etc. Should have built in logbook for recording events li				
Uptake time should be a minimum of 90%. Proof of locally available technical support personnel, including CVs and work permits for foreign personnel. Availability of technical personnel within the country should be stated; this should include CVs, work permits for foreign personnel. Software should be flexible and provide the room for upgrade to add new parameters to be measured by the Machine and report format. Documentation: Operating and service manuals (In English) including lists of important spares and accessories - with their part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007-Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation of Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and long (Pressureoune, volume flow and pressure-flow) pulmonary graphics Digital display of FlO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous				-
Proof of locally available technical support personnel, including CVs and work permit for foreign personnel. Availability of technical personnel within the country should be stated; this should include CVs, work permits for foreign personnel. Software should be flexible and provide the room for upgrade to add new parameters to be measured by the Machine and report format. Documentation: Operating and service manuals (In English) including lists of important spares and accessories - with their part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit INW/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (Size 4f) for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphirs Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expristory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C2O/C), ung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms, integrated monitoring, integrated volume and pressure monitoring i				die.
CVs and work permit for foreign personnel. Availability of technical personnel within the country should be stated; this should include CVs, work permits for foreign personnel. Software should be flexible and provide the room for upgrade to add new parameters to be measured by the Machine and report format. Documentation: Operating and service manuals (in English) including lists of important spares and accessories - with their part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit INV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/ASSist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peab pressure, mean airway pressure, CPAP/PEEP, Expiratory fidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/c), Lung time constant, Rate volume ratio etc. Should have built in logbook for recording events like various alarms, integrate				
Availability of technical personnel within the country should be stated; this should include CVs, work permits for foreign personnel. Software should be flexible and provide the room for upgrade to add new parameters to be measured by the Machine and report format. Documentation: Operating and service manuals (In English) including lists of important spares and accessories - with their part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit INM/JPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low ast-2-ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, John and pressure-flow) pulmonary graphins Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms, integrated monitoring, Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspon		13		
Adjustable Mayo table				
Adjustable Mayo table Adjustable Mayon tabl				
Adjustable Mayo table Documentation: Operating and service manuals (in English) including lists of important spares and accessories - with their part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilation design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low ast-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various elarms, integrated monitoring in fergrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTSpont, My and Myleak. The volume monitoring should have N1PD to BTPS correction. Monitoring			Programme and the second se	
add new parameters to be measured by the Machine and report format. Documentation: Operating and service manuals (In English) including lists of important spares and accessories - with their part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low ass1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, eman airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, ung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. integrated monitoring integrated volume and pressure monitoring ie. monitoring of PEEP Pmax, Pmean and VT, VTSpont, MV and MVleak. The volume monitoring feet pressure and Spont.			I to the second of the second	
format. Documentation: Operating and service manuals (In English) including lists of important spares and accessories - with their part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low ast-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of Fi02, Peak pressure-flo			I the control of the	
Documentation: Operating and service manuals (in English) including lists of important spares and accessories - with their part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, ung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms, integrated monitoring, Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NIPD to BTPS correction. Monitoring of ie. Frequency and Spont.	222	Adjustable Mayo		
including lists of important spares and accessories - with their part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: tife span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TET medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure, flow) pulmonary graphirs Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. integrated monitoring, Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MY and MVleak. The volume monitoring should have NIPD to BTPS correction. Monitoring of ie. Frequency and Spont.	30			
part numbers and list of equipment and procedures required for calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) puimonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring, Integrated volume and pressure monitoring i.e. monitoring should have NIPD to BTPS correction. Monitoring of PEEP Pmax, Pmean and VT, VTspont,				
calibration and routine maintenance should be provided. Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: tife span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilations IMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, eman airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C2O/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NIPD to BTPS correction. Monitoring of ie. Frequency and Spont.				in .
Documentation must also show recommended procedures for disposal and any probable hazards to the environment and/or community. Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure, Elow) pulmonary graphirs Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compfiance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring. Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NIPD to BTPS correction. Monitoring of ie. Frequency and Spont.		W. W.		
disposal and any probable hazards to the environment and/or community. Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As per ISO J4971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C2O/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring. Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NIPD to BTPS correction. Monitoring of ie. Frequency and Spont.				
community. Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak prossure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring, Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NIPD to BTPS correction. Monitoring of ie. Frequency and Spont.				
Life span: Life span of the machine should be not less than 10 Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphirs Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have N1PD to BTPS correction. Monitoring of ie. Frequency and Spont.				"
Years. Risk Classification: As per ISO 14971:2007- Application of risk management to medical devices. Regulatory Approval / Certification: TAEC, TBS and TFDA The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms, integrated monitoring. Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NIPD to BTPS correction. Monitoring of ie. Frequency and Spont.	•		1 33 · · · · · · · · · · · · · · · · · ·	
The Ventilator should be microprocessor controlled designed for neonatal use. There should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms, integrated monitoring, Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NIPD to BTPS correction. Monitoring of ie. Frequency and Spont.	 			
The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphirs Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C2O/C), tung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring. Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NIPD to BTPS correction. Monitoring of ie. Frequency and Spont.			Risk Classification: As per ISO 14971:2007- Application of risk	1
The Ventilator should be microprocessor controlled designed for neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C2O/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NIPD to BTPS correction. Monitoring of ie, Frequency and Spont.		W Committee	management to medical devices.	15
neonatal use. There should be possibility to upgrade with additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C2O/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NTPD to ETPS correction. Monitoring of ie. Frequency and Spont.			Regulatory Approval / Certification: TAEC, TBS and TFDA	
additional features Continuous flow, pressure limited, time cycled ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C2O/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have N1PD to BTPS correction. Monitoring of ie. Frequency and Spont.			The Ventilator should be microprocessor controlled designed for	
ventilator design Ventilator modes: should have following modes available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphirs Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NTPD to BTPS correction. Monitoring of ie. Frequency and Spont.			neonatal use. There should be possibility to upgrade with	
available in the unit IMV/IPPV CPAP including non-invasive ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C2O/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NTPD to BTPS correction. Monitoring of ie. Frequency and Spont.			additional features Continuous flow, pressure limited, time cycled	
ventilation SIMV, SIPPV/Assist-control Volume targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C2O/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NIPD to BTPS correction. Monitoring of ie. Frequency and Spont.			ventilator design Ventilator modes: should have following modes	
targeted/guarantee mode of ventilation with ability to deliver and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring. Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NTPD to BTPS correction. Monitoring of ie. Frequency and Spont.			T	
and monitor tidal volume as low as1-2ml (Range 2ml to 50 ml) Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring. Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NTPD to BTPS correction. Monitoring of ie. Frequency and Spont.		V.		
Pressure support mode of ventilation Apnea back-up ventilation Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NIPD to BTPS correction. Monitoring of ie, Frequency and Spont.				
Should have integrated high resolution TFT medical grade screen (size 4") for real time display Scalar (Pressure, Flow and Volume against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring. Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NTPD to BTPS correction. Monitoring of ie. Frequency and Spont.			1 · · · · · · · · · · · · · · · · · · ·	
Neonatal ventiliator				
Neonatal ventiliator against time) and loop (Pressurevolume, volume flow and pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have N1PD to BTPS correction. Monitoring of ie. Frequency and Spont.				
pressure-flow) pulmonary graphics Digital display of FiO2, Peak pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C2O/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have N1PD to BTPS correction. Monitoring of ie. Frequency and Spont.				
pressure, mean airway pressure, CPAP/PEEP, Expiratory tidal volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NIPD to BTPS correction. Monitoring of ie. Frequency and Spont.	31	Neonatal ventillator		
volume, expiratory minute volume, total frequency, spontaneous frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NTPD to BTPS correction. Monitoring of ie. Frequency and Spont.				
frequency, lung function monitoring Compliance, resistance, lung distention coefficient, (C20/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NTPD to BTPS correction. Monitoring of ie. Frequency and Spont.				
distention coefficient, (C2O/C), Lung time constant, Rate volume ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NTPD to BTPS correction. Monitoring of ie. Frequency and Spont.				
ratio etc. Should have built-in logbook for recording events like various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NTPD to BTPS correction. Monitoring of ie. Frequency and Spont.				
various alarms. Integrated monitoring: Integrated volume and pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NTPD to BTPS correction. Monitoring of ie. Frequency and Spont.			I 01	
pressure monitoring i.e. monitoring of PEEP Pmax, Pmean and VT, VTspont, MV and MVleak. The volume monitoring should have NTPD to BTPS correction. Monitoring of ie. Frequency and Spont.			i i i i i i i i i i i i i i i i i i i	
VT, VTspont, MV and MVleak. The volume monitoring should have NTPD to BTPS correction. Monitoring of ie. Frequency and Spont.				
BTPS correction. Monitoring of ie, Frequency and Spont.				
BTPS correction. Monitoring of ie, Frequency and Spont.			MV and MVleak. The volume monitoring should have NTPD to	
Frequency Settings range: Trigger Flow/volume, leak	1		la contraction of the contractio	
The state of the s	133		Frequency Settings range: Trigger Flow/volume, leak	

34	Cardiac table	 Size:900*450*900-1200mm Wooden dinning board(800*400mm) Steel frame, ABS gas spring bottom Height is adjustable, controlled by gas-spring Four silent castors, φ55mm 	
33	Bedside lockers	 dimension 520*480*740 made of high density wood one drawer and one door with handles, top with rail two tower hanger, four wheels with cross breaks 	
32	Patient Beds with mattress,	Bacterial filters 50 sets Flow sensors 20 sets Oxygen cell and Oxygen connecting hose Air connecting hose Battery back-up (at least 30 minutes) • Heavy duty bed Size (L*W*H): 2150*950*500mm • High quality section steel welding • The surface electrostatic sprayed • Corrosion resistant • Easy to clean • Side guard made of well plastic • I.V pole • Four casters, two caster with brakes	
		adapted PIP 8 to 80cm of water PEFP/CPAP 0 to 25 mbar Five years comprehensive Maintenance inclusive. I:E ratio 1:0 to 1:10 Inspired Time 0.1 to 2 sec Expired Time 0.2 to 30 sec Frequency Up to 200 BPM Base Flow (VIVE) 1 to 30 LPM Synchronization Patient synchronization Integrated blender for Oxygen 21 % to 100% Integrated nebulization facility Integrated screen for display of Pressure-Time, Flow-Time and Volume-Time curves Integrated monitoring of FiO2 Monitoring of flow: At the Y piece with facility to activate it Audiovisual alarms with advisory on-screen message: MV high/low, Apnea, tube obstruction, FiO2, high/low high PIP, low PEEP/CPAP, fail to cycle, gas supply low, power failure, ventilator inoperative, alarm log book. The ventilator should have automatic compensation for leakage and should monitor and display leakages The ventilator should show trends of important parameters viz. C,R, FiO2, MAP, etc for evaluation of patient improvement Power Supply: 220 - 240V, 50Hz. SCOPE OF SUPPLY Ventilator on trolley with wheels and brake facility Integrated medical air compressor Humidifier with autoclavable chamber and complete with patient circuit support arm Nebulization accessories (2 sets)	

		Wall Mounted Oxygen Flowmeter with Humidifier Oxygen Flowmeter with Humidifier is suitable for concentrated oxygen supply system in hospitals.	
35	Oxygen Flow meter	Main performances: Flow range: 015L/min. Automatic exhaust pressure of safety valve: 0.35±0.05 MPa; This unit should adopt British standard should be equipped with humidifier bottle that can be autoclavable at 120 centigrade.	
39	Apheresis machine	Should have starter pack, Desktop, workstation, UPS750, ups 10KVA, Access control, server, data carbonate, router, switch, LANaccessories, and installation Lumpsum. Construction material: Sheet metal Voltage 100-240 V (±10%; switch selectable) Frequency 50/60 Hz Centrifuge speed 3000-7000 rpm (varies with protocol) Pump speed Draw: 20-100 mL/min Return: 20-140 mL/min, Five years comprehensive Maintenance inclusive.	
40	Plasma Apheresis machine	Power supply (V/Hz) - 220-/50 Amount collected per cycle (g) - 0-300 Total plasma collection (g) - 0-1000 Pump speed (ml/min) - 20-100 Return speed (ml/min) - 20-100 Anticoagulant (Citrate) to whole blood ratio - 1:12-1:16 Centrifuge speed (r/mim) - 7000. Five years comprehensive Maintenance inclusive.	
41	Gene Sequencing	Desktop Sized Sequencing Instruments - "Next-Next Generation Sequencing" • Scaled down • Medium throughput •able to analyse COVID and Cancer markers, • Should be supplied with start up consumables • Unit should function with 220-240Vac, 50 Hz input power supply. • Unit should be supplied with suitable UPS with a minimum 30 minutes back-up time.	

Should have facility for Invasive and Non-Invasive ventilation Microprocessor Control suitable for Pediatric and Adult ventilation Electromagnetic Compatible Hinged arm holder for holding the circuit Should have built-in touch colour screen TFT display of minimum 10 inches or more for display of waveforms and Monitored value, Five years comprehensive Maintenance inclusive. Should have in-built facility to upgrade with EtcO2	42 ICU Beds	corners Handset, ACP Box, Battery Back Up, SMPS Bed Extension, Linen Holder, Night Lamp, Angle Indicator.Polymer -Moulded Head and Foot Panels (Removable) - Polymer Moulded Split Safety Rails (2 sets) Urine Bag Holder (Single) S.S Heavy Duty I.V. Pole (2 hooks) Premium mattress, single section, 4", with wave shape on both sides, High quality, high density, flame retardant foam and cover fabric having flame retardant, antibacterial, antiskid properties Mattress for Bed Extension	
ventilation Electromagnetic Compatible Hinged arm holder for holding the circuit Should have built-in touch colour screen TFT display of minimum 10 inches or more for display of waveforms and Monitored value, Five years comprehensive Maintenance inclusive.		· ·	
		ventilation Electromagnetic Compatible Hinged arm holder for holding the circuit Should have built-in touch colour screen TFT display of minimum 10 inches or more for display of waveforms and Monitored value, Five years	

KAS MEDICS LIMITED

Your partner in progressive healthcare

70

Secretary,
MZRH Tender Board,
P. O. Box 419,
Mbeya, Tanzania.



Date: 26th November, 2021 IFT NO. ME/007/MBY/2021/22/CS/MV/09

냶
ΙŻ
IR
120
IB
>
12
15
먇
IΞ
IZ
12
I≥
TENDER FOR SUPPLY INSTALLATION, TESTING COMMISSIONING AND TRA
15
ΙÖ
2
2
ΙĘΙ
1ត
lo.
10
I≨
I≦
S
Ιō
ΙZ
ΙZ
G A
15
15
15
Έ
ΙZ
ਙ
AINING OF A
13
ı≥.
므
Q
=
EDICAL EQ
몯
1=
S
罗
=

7	15	14	13	12	11	10	9		DO	~	6	15	4	ω				2	jud.		
-	33	31	30	29	28	19	7		ō.	(J)	4	La Carte	2	1	icu	ITEM#	LOT NO	2	ы	ПЕМ#	LOT NO.
Dual-tube laryngeal mask airway(LMA) (#2 - 7)	Drip stand	Digital thermometer (32 - 42) CLINICAL THERMOMETER)	Delivery set	Defibrillator with pacing capabilities	Defibrillator pads	Child weighing scale (250g graduation)	Bed pans Stainless steel	pressure limiting valve,	Bag-valve-mask Ambu Oval Plus Silicone Resuscitator, Adult, with patient valve,	Automated external defibrillator (AED)	Autoclave (electric or non-electric) and supplies	ARTERIAL BLOOD GAS (ABG) MACHINE	HEAVY DUTY MECHANICAL VENTILATOR	STANDARD ICU Beds		ПЕМ	2. SONGWE RRH.	DIGITAL X-RAY	CT SCAN MACHINE 64 SLICES WITH INSTALLATION AND 5 YRS MAINTANANCE PLAN	пем	LOT NO. 1. SUPPLY OF PHILIPS MEDICAL EQUIPMENT
SET/6	Ea	Еa	Ea	£a	Pairs	Eа	Ea		Ea	Ea	£a	Ea	Ea	Ea		NoU		EA	EA	MoU	
50	8	6	3	1	20	1	co		10	2	j.a	1	4	12		QTY		5	9	QTY	
	SKH041-4		SET 201	HD-7			03.8336 BED PAN ADULT PERFECTION TYPE		470 017 100	FRED PA-1	YX-280D 18L	115	Gradian CCV	080		MODE/CAT No		FMT	SUPRIA 64/128	MODE/CAT No	
AMBU	SAIKANG	FAZZINI	FAZZINI	SCHILLER	SCHILLER	ARI MEDICAL TECHNOLOGIES	FAZZINI	AMBU		SCHILLER	ARI MEDICAL TECHNOLOGIES	EDAN	GRADIAN HEALTH	SAIKANG		BRAND/MANUFACTUR ER		DEL MEDICAL	HITACHI/FUJIFILM	BRAND/MANUFACTUR ER	č
150,000.00	100,000.00	10,000.00	1,200,000,00	22,500,000,00	450,000,00	200,000.00	350,000.00	410,000.00		3,500,000.00	910,000.00	19,000,000.00	28,000,000.00	6,750,000.00		Unt Price		290,000,000.00	1,800,000,000.00	Unt Price	
7,500,000.00	800.000.00	60,000.00	3,600,000.00	_22,500,000.00	9,000,000.00	200,000.00	2,800,000.00		4,100,006.00	00.000,000	00.000,010	19,000,000 up	112 000 000 00	40 Jug Dug B	1 - 4	tine Total		1,450,000,000.00	10,800,000,000,00	Line Total	

48	47	46	45	44	43		42	41	40	99	S IS	3/	36	35	34	33	32	31	30	29	87	27	26	25	24	23	22	21	20	19	18	17				16		
2/	26	25	25	5	4	EMD	93	91	a v	84	3	82	81	80	79	78	77	75	74	73	12	70	19	60	57	98	47	46	38	33.7	36	35			Ī	34		
Delivery set	Defibrillator with pacing capabilities	Defibrillator pads	Crash Trolley (cart)	Automated external defibrillator (AED)	Autoclave (electric or non-electric) and supplies		Patient Beds with matress	X-ray viewing box or digital system	Portable Ultrasound machine	Surgical cricothyroidotomy set	Suction device: powered (electric or pneumatic)	Suction device: manual (bulb) or foot pump	Stretchers and gurneys (wheeled stretchers)	Stethescope	Sterile gauze drum	Sterile dressings drum	Specimen containers (STOOL/URINE CONTAINER)	Safe final disposal of sharps (SAFETY BOX)	Safe biological waste disposal containers (SAFETY BOX)	Refrigerator with thermometer	Pulse oxymetry	Patient Wheelchairs	Nebulizer machine (HEAVY DUTY PROFESSIONAL NEBULIZER)	Nebulization masks (pediatric and adult sizes)	N-95 respirators	Mechanical Ventilator	Glucometer test strips	GLUCOMETER	Electronic multi-parameter cardiac monitor	ECG electrodes (DISPOSABLE ELECRODES)	ECG paper (A4 SIZE, Z-FOLD)	PORTABLE ECG MACHINE	Ambu AuraGain Size 6	Ambu AuraGain Size 5	Ambu AuraGain Size 4	Ambu AuraGain Size 3	Ambu AuraGain Size 2½	Ambu AuraGain Size 2
Еà	Ea	Pairs	Ea	Ea	Ea		E3	Ea	Ea	Ea	Ea	Ea	Еa	£а	Ea	Ea	Ea	Eа	Ea	Ea	Ea	Ea	Ea	50pcs	Ea	Ea	Ea	Ea	Ea	Ea	Rolls	£a				_		
ω	1	10	4	1	<u>, , , , , , , , , , , , , , , , , , , </u>		12	2	2	4	4	2	4	6	3	3	100	100	- 6	1	6	б	2	4	500	2	50	w	2	1000	20	1		Ī				
SET 201	HD-7		SK-ET75077A	FRED PA-1	YX-280D 18L		A1K	SK-L516	MyLab Sigma (PORTABLE ECHO ULTRASOUND)		F-30.65/PF	F-175	SKB041-3S							YY-800	BT710	9001 ŞTEEL WHEELCHAIR	F-210 PRC	05,5009/05,5010	N95	Gradian CCV	GLUCO-DR AUTO STRIPS	GLUCO-DR AUTO (AG4000)	iM80 with 12 lead ECG			SE-1200	408600000	408500000	408400000	408300000	408250000	408200000
FAZZINI	SCHILLER	SCHILLER	SAIKANG	SCHILLER	ARI MEDICAL TECHNLOGIES		SAIKANG	SAIKANG	ESAOTE		FAZZINI	FAZZINI	SAIKANG	FAZZINI	FAZZINI	FAZZINI		KARTEL	KARTEL	SYSMEDICAL	BISTOS	ARI MEDICAL TECHNOLOGIES	FAZZINI	FAZZINI	3M	GRADIAN HEALTH	ALLMEDICUS	ALLMEDICUS	EDAN	AMBU	SCHILLER	EDAN						
1,200,000 00	22,500,000.00	450,000.00	2,000,000.00	3,500,000.00	910,000.00		90,000,00	850,000.00	64,000,000.00	1,000,000.00	1,800,000.00	570,000,00	2,500,000.00	70,000 00	300,000.00	300,000,00	300.00	3,500,00	3,500.00	4,900,000.00	00'000'056	350,000.00	600,000.00	250,000.00	5,000.00	28,000,000.00	25,000.00	25,000.00	9,000,000.00	130.00	30,000,00	5,875,000.00						
3,600,000 00	22,500,000.00	4,500,000.00	8,000,000.00	3,500,000.00	910,000.00	•	10,800,000,00	1,700,000.00	128,000,000.00	4,000,000.00	7,200,000.00	1,140,009,00	10,000,000.00	420 000 00	900,000.00	900,000,00	30,000,00	350,000,00	21,000.00	4,900,000.00	5,700,000.00	2,100,000.00	1,200,000.00	1,000,600.00	2,500,000.00	56 000 000 00	1,250,000.00	75,600.00	18,000,000.00	130,000.00	600,000.00	5,875,000,00						

72	71		į			70	69	88	67	66	65	54	2	63	62	51	60	59	58		Sec.		57	56	55	54	S3	52	51	50	49
2	μå	EMD	TEM#	LOT No.		88	87	86	84	81	78		77	76	70	66	55	54	51				47	40	39	34	33	32	31	29	28
Portable cardiac monitor monitors with movable stand	Heavy duty mechanical ventilator with neonatal, infants, children and adult function		ПЕМ	3 MBEYA ZONAL REFERRAL HOSPITAL		WHEEL chair	Bedside lockers	Patient Beds with matress	X-ray viewing box or digital system	Portable Ultrasound machine	Suction machine: powered (electric or pneumatic)	SKM-G Hydraulic patient trolley	Heavy duty Stretchers	Stethescope	Refrigerator with thermometer	Patient Wheelchairs	Nebulizer machine	Nebulization masks (pediatric and adult sizes)	N-95 respirators	100071 FIBER-OPTIC MILLER LARYNGOSCOPE COMPLETE MATT TYPE W\3 S.S.BLADES SIZE 00,0,1 W/CARRYING CASE 97.60 + 100065 FIBER-OPTIC HANDLE FOR CHILD	+ 100017: LARYNGOSCOPE HANDLE FOR ADULT MATT TYPE	100027 McINTOSH LARYNGOSCOPE COMPLETE MATT TYPE W/4	Laryngoscope set (range of blades and sizes)	Glucometer test strips	GLUCOMETER	Electronic multi-parameter cardiac monitor.	ECG electrodes (DISPOSABLE ELECRODES)	ECG paper	ECG MACHINE	Drip stand	Digital thermometer (32 - 42)
Ea	Ea		UoM			Ea	Εa	Ea	Ea	Eа	Ea		Ea	Ea	Ea	Ea	Еà	Ea	Ea				E3	Ea	E	Ea	Ea	Rolls	Ea	Ea	Ea
2	1		QTY			6	12	12	1	2	4		10	6	1	6	2	20	500				2	50	3	2	100	20	ь	8	10
iM70 with movale stand	U-VENT		MODE/CAT No			9001 STEEL WHEELCHAIR	SK5002	A1K	SK-L516	MyLab Sigma (PORTABLE ECHO ULTRASOUND)	F-30.65/PF		SKB041-35		YY-800	9001 STEEL WHEELCHAIR	F-210 PRO		N95	100071 100065	10001/	100027		GLUCO DR. AUTO STRIPS	GLUCO DR. AUTO (AG 4000)	iM80 with 12 lead ECG			SE-1200	SKH041-4	
EDAN	UTAS		BRAND/MANUFACTUR ER			ARI MEDICAL TECHNOLOGIES	SAIKANG	SAIKANG	SAIKANG	ESAOTE	FAZZINI		SAIKANG	FAZZIN	SYSMEDICAL	ARI MEDICAL TECHNOLOGIES	FAZZINI		3M				FAZZINI	ALLMEDICUS	ALLMEDICUS	EDAN	SCHILLER	SCHILLER	EDAN	SAIKANG	FAZZINI
5,000,000.00	55,000,000.00		Unt Price			350,000.00	200,000.00	900,000,00	850,000.00	64,000,000.00	1,800,000.00		2,500,000.00	00.000,07	00.000,000,8	00.000,028	600,000.00		5,000.00				1,800,000 00	25,000.00	25,000.00	00.000,000,0	2,000.00	30,000.00	5,875,000,00	100,000.00	10,000,00
10,000,000.00	55,000,000.00	4	Line Total		4 7	2,100,000.00	2,400,000.00	10,800,000.00	850,000.00	128,000,000.00	7,200,000.00		25,000,000.00	420,000.00	6,000,000.00	2,100,000.00	1,200,000.00	•	2,500,000.00				3,600,000.00	1,250,000.00	75,000.00	18,000,000.00	200,000.00	600,000,00	5.875,000.00	800,000.00	100,000,00

Г	96	95	94	90	89	00			9	97 0	a c	P 9		83	82	81	80	79	78	77	76	3	75	74	73
	43	42	40	87	24	23			1.2	2 6	19	17	6	ň	13	12	11	10	9	89	-4	6	-	л	3
(startup consumables and 1 set of reagents included)	5-Part-Diff Fully Automatic Hematology analyzer Support whole blood and capillary blood sample, U graphs, Westgard rules, NRBC,RETICs count, Clot detection	ruly automatic Clinical chemistry Analyzer with minimal reaction volume, capable of electrolytes testing. U Graphs, westgard rules, clots detection, Built in bar code reader.	Apheresisimachine	Portable X-ray machine	Video laryngoscope	Vein finder	ADDUZZ HBER-OPTIC MILLER LARYNGOSCOPE COMPLETE MATT TYPE VX\3 S.5. BLADES SIZE 00,0,1 W/CARRYING CASE 97.60 + 100065 FIBER-OPTIC HANDLE FOR CHILD	+ 100017: LARYNGOSCOPE HANDLE FOR ADULT MATT TYPE	100027 McINTOSH LARYNGOSCOPE COMPLETE MATT TYPE WA	propor waterier	Infusion pump	Wheel chairs	SKM-G Hydraulic patient trolley	Heavy duty stretchers	Defibrillator pads	Defibrillator with pacing capacity	Heavy duty oxygen concentrator High flow (10-15/min)	Heavy duty electrical suction machine	ECG disposable electrodes	ECG machine with 12 led electrodes and fixed movable stand	Portable USS with abdominal, cardiac and linear probe and movable stand	"SKM-B Emergency trolley	"SKM-B Emergency trolley	Emergency trolley	Multi parameter cardiac monitors with wall mounting flex bie stand(Philips brand)
	Each	Each	Ea	Ea	Ea	E a			Ea	Ea	Ea	Ea	Ea		Pairs	Ea.	Ea	Еa	Ea	Fa	e3	Ea	Ea		Ea
		þ	ш	٢	1	ω			VI	2	4	tά	20		20	2	2	ш	5000	-	L	45	ω		ر. د
	SH-H2	BA 200	XI:	MDR	(Discposable Blades)	QV-500	100071	100027		FT1800	AIP-1200	9001 STEEL WHEELCHAIR		SKB041-3S		HD-7	OLV-10 DUO FLOW	F-100	1 2 2 2 2 2 2 2 2 2 2 2 2 2 2 2 2 2 2 2	SE-1900	MyLab Sigma (PORTABLE	SK-ET75077A	SK-ET75077A		iM70 with wall mounting
	ARTEMISLIFE	BIOSYSTEM	Qingdao Haier Biomedical Co., Ltd.	DEL MEDICAL	AMBU	ARI MEDICAL TECHNOLOGIES			FAZZINI	BIO-X	ARI MEDICAL TECHNOLOGIES	ARI MEDICAL TECHNOLOGIES		SAIKANG	SCHILLER	SCHILLER	ZZ-0LIVE	£A77INI	SCHILLER	no.	ESAOTE	SAIKANG	SAIKANG	EUAN	CDAN
	45,000,000 00	65,000,000.00	51,000,000.00	290,000,000,00	9,500,000.00	3,500,000,00			1,800,000.00	5,000,000.00	1,900,000.00	350,000.00		2,500,000.00	450,000.00	22,500,000,00	5,000,000,00	00,000,00	00,000,00	20000	64,000,000.00	2.000.000 00	2,000,000.00	9,500,000,00	200 000 00
	45.000,000.00	65,000,000.00	51,000,000.00	290,000,000.00	9,500,000.00	10,500,000.00			9,000,000.0	10,000,000,00	7,600,000.00	3,500,000.00	50,000,000.00		9,000,000,00	45,000,000,00	10,000,000,00	00.000,000,01	2,672,000.00		64,000,000.00	8,000,000,00	6,000,000 00		24,500,000.00

126	125	124	123	122	121	120	119			118	117	116	115	114	113	112	111	110	109	108	107	106	105	104	103	102	101	100	99	86	37
51	48	47	45	44	41	40	36		83		32	30	28	27	26	25	24	23	22	21	18	15	14	12	11	9	œ	5	4	ICU	
Spirometry	Bed pan	Nebulizer machine	Drip stands	Heavy duty stretcher	Nebulizer Machine	Wall pipe oxygen flow meter	Vein finder	100071 FIBER-OPTIC MILLER LARYNGOSCOPE COMPLETE MATT TYPE W/3 S.S.BLADES SIZE 00,0,1 W/CARRYING CASE 97.60 + 100065 FIBER-OPTIC HANDLE FOR CHILD	100027 McINTOSH LARYNGOSCOPE COMPLETE MATT TYPE W\4 S.S.BLADES SIZE 0,1,2,3, and 2 spare bulbs, W/CARRYING CASE + 100017: LARYNGOSCOPE HANDLE FOR ADULT MATT TYPE	Laryngoscope set (range of blades and sizes)	Videa laryngoscope	Infusion pump	Heavy duty stretchers	Defibrillator pads	Defibrillator with pacing mode	Heavy duty oxygen concentrator High flow (10-15/min)	Heavy duty electrical suction machine	EGC disposable electrodes	ECG machine with 12 electrodes with fixed movable stand and disposable electrodes	Portable USS with abdominal, cardiac and linear probe and movable stand	ABG(Blood gases machine with reagents)	Multi-parameter cardiac monitors with wall mounting flexible stand	Portable cardiac monitor monitors with movable stand	Breathing circuit	HME bacteria filter	Heavy duty mechanical ventilators	Bedside lockers	ICU beds with CPR capabilities (CPR board) and air matrices	Digital Portable x-ray		
E3	Ea	Ea	Ea	Ea	Ea	Ea	Ea			E3	Ea	Ea	Ea	Pairs	Ea	£а	Ea	Ea	63	Ea	Ea	Ea	Ea	Ea	Ea	Ea	Ea	Еа	63		
20	26	2	26	12	2	26	2			10	1	26	2	40	2	2	. 26	10,000	1	1	1	20	2	200	300	16	26	26	1		
SPIROVIT SP-1	03,8336 BED PAN ADULT PERFECTION TYPE	F-210 PRO	SKH041-4	SKB041-3S	F-210 PRO		QV-500	100071 100065	100027	55	KingVision with a Blade (Discposable Blades)	AIP-1200	SKB041-3S		HD-7	OLV-10 DUO FLOW	F-100		SE-1200	MyLab Sigma (PORTABLE ECHO ULTRASOUND)	115	iM70 with wall mointing	iM70 with movale stand			Gradian CCV	SK5002	D8D	MDR		
SCHILLER	FAZZINI	FAZZINI	SAIKANG	SAIKANG	FAZZINI	ARI MEDICAL TECHNOLOGIES	ARI MEDICAL TECHNOLOGIES			FAZZINI	AMBU	ARI MEDICAL TECHNOLOGIES	SAIKANG	SCHILLER	SCHILLER	ZZ-OLIVE	FAZZINI	AMBU	EDAN	ESAOTE	EDAN	EDAN	EDAN	GRADIAN HEALTH	GRADIAN HEALTH	GRADIAN HEALTH	SAIKANG	SAIKANG	DEL MEDICAL		
6,400,000,00	350,000.00	600,000.00	100,000.00	2,500,000.00	600,000.00	150,000.00	3,500,000.00			1,800,000.00	9,500,000.00	1,900,000.00	2,500,000.00	450,000.00	22,500,000.00	5,000,000.00	2,800,000.00	2,000.00	00.000,278,2	64,000,000.00	19,000,000.00	4,900,000.00	5,000,000.00	130,000.00	10,000,00	28,000,000.00	200,000.00	6,750,000.00	290,000,000.00		
128,000,000.00	9,100,000.00	1,200,000.00	2,600,000.00	30,000,000.00	1,200,000.00	3,900,000.00	7,000,000.00			18,000,000.00	9,500,000.00	49,400,000.00	5,000,000.00	18,000,000.00	45,000,000.00	10,000,000.00	72,800,000.00	20,000,000.00	5,875,000.00	64,000,000.00	19,000,000.00	98,000,000.00	10,000,000.00	26,000,000,00	3,060,000.00	448,000,000.00	5,200,000.00	175,500,000.00	290,000,000.00		,

C47	1444	140	142	1 12	140	139	138	1	137	136	1261		-				104		122	2 1	130	129			T		128	127	
38	ť	200	3 6	3 12	21	20	19		16	15 t	3				11		u	1	α -	7	4	2	EMD	ITEM#	LOT No.	4.5	2		52
Deflibrator machine with pacing capacity	Naouilzer machine	Nebulizer mask	neingerator with regulator thermometer	Wayo table	Portable ultrasound machine with abdominal, cardiac and linear probe	Saans CPAP + HFNC Device (NEONATE) Including: Humidifer + Trolley + startup disposoble consumables (i.e Saans Ram's Cannula Size 1, Saans Ram's Cannula Size 0, Saans Disposable CPAP & PIP Circuit, Saans Mask (Neonatal Size 0)	Portable mechanical ventilator with pediatrics and adult functions CPAP machine	Separation and a republication of the separation	Portable cardiac monitor with a leade electrodor	Heavy dirty stratcher	* LOUGES FIBER-OFFIC HANDLE FOR CHILD	VA3 5.5.BLADES SIZE 00,0,1 W/CARRYING CASE 97.60	100071 FIBER-OPTIC MILLER LARYNGOSCOPE COMPLETE MATT TYPE	+ 100017: LARYNGOSCOPE HANDLE FOR ADULT MATT TYPE	ISS BIADES SIZE 0.1.2.3 and 2 space bribs (W/CARRYY)C CASE	Laryngoscope set (range of blades and sizes)	examination light	Outoclave Hidenine (22 t) (ERS)	Autoclaro machine (300 WA75)	Operating table JAC-A trectric operating table)	Reavy Suction machine	Vein finder		ПЕМ	. 4: Songea Regional Referral Hospital	e-guer puriatre x-ray		100071 FIBER-OPTIC MILLER LARYNGOSCOPE COMPLETE MATT TYPE IVA3 S S.BLADES SIZE DO, D.1 W/CARRYING CASE 97, 60 + 100063 FIBER-OPTIC HANDLE FOR CHILD	Fibreoptic flexible laryngoscope
EA	EA	50pcs	ΕA	ΕA	ΕA	EA	EA	EA	E A	EΑ						Ea	ĒΑ	ĒΑ	ΕA	ΕA	EA	EA		MoU		£a	200		Ea
	2	50	ļ.	5	1	ν.	2	4	6	2						4	- 6	2	4	1	4	2		QTY		-			4
HD-7	F-210 PRO	05.5009/05.5010	YY-800	SKH038-2	MyLab Sigma (PORTABLE ECHO ULTRASOUND)	F2-01-000-00-000	Gradian CCV	IM70 with mobile trolley	SKB041-3S	FRED PA-1	TOGGGG	100071		100017	100027		02,738.00	NC 32	DIATROM 300	A301	F-100	QV-500		MODE/CAT No		MDR		100065	100071
SCHILLER	FAZZINI	FAZZINI	SYSMEDICAL	SAIKANG	ESAOTE	SAANS	GRADIAN HEALTH	EDAN	SAIKANG	SCHILLER						FAZZINI	FAZZINI	NUVE	FAZZINI	SAIKANG	FAZZINI	ARI MEDICAL TECHNOLOGIES	EK	BRAND/MANUFACTUR		DEL MEDICAL			FAZZINI
22 500,000,00	600,000,00	250,000.00	6,000,000.00	300,000.00	64,000,000.00	15,000,000.00	28,000,000.00	5,000,000.00	2,500,000.00	3,500,000.00						1,800,000,00	750,000,00	19,000,000,00	16,000,000.00	15,000,000,00	2,800,000,00	3,500,000.00		Unt Price		290,000,000.00			4,500,000.00
22,500,000 00	1,200,000.00	12,500,000.00	6,000,000.00	1,500,000.00	64,000,000.00	30,000,000.00	56,000,000.00	20,000,000.00	15,000,000.00	7,000,000.00					1100,000,00	7,200,000,00	4 500,000,00	OU DOU DOU BE	64,000,000.00	15,000,000 00	11.200.000.00	7,000,000.00		Line Total	,	290,000,000.00		Ĭ.	

	3 5	1/0		169	168	167	166	165	164	163	162	160					159	158	į,	156	155	154	152		151	149	T		148	147	
0.0	70/	53	46		35	34	33	32	30	29	28	A 10	EMD	ITEM#	LOT No		26	24 2		21	20	19	17		16	μ μ	ē		41	40	
Secure	Reingerator with thermometer	Nebulizer machine	100027 McINTOSH LARYNGOSCOPE COMPLETE MATT TYPE W/4 5.S.BLADES SIZE 0,1,2,3, and 2 spare bulbs, W/CARRYING CASE + 100017: LARYNGOSCOPE HANDLE FOR ADULT MATT TYPE 100071 FIBER-OPTIC MILLER LARYNGOSCOPE COMPLETE MATT TYPE W/3 5.S.BLADES SIZE 00,0,1 W/CARRYING CASE 97.60 + 100065 FIBER-OPTIC HANDLE FOR CHILD	Laryngoscope set (range of blades and sizes)	Electronic malt parameter cardiac monitor with 5 electrodes	ECG paper	ECG disposable electrodes	ECG machine with 12 lead electrodes	Drip Stand	Digital thermometer (3) - A3 Calcine) CHAICAL TUEBAACAACTER	Defibrilator with paring capabilities	Autoclave (electric or non-electric) and supplies		ITEM	LOT No. 5 SUMBAWANGA REGIONAL REFERRAL HOSPITAL		Nebulizer machine	function Heavy ditty stratcher	Heavy Mechanical ventilator ventilator with pediatric and adult	Heavy oxygen concentrator	Heavy suction machine (electric)	Defibrillator with paring canability	Infusion pump	Day strike year	ARG pas analyzer	Standard ICU beds WITH CPR capability			ECG disposable electrodes	ECG machine	
Ea	Ea	E3		Ea	Ea Cont	Rolls	E a	2 5	5 0	Ea	Ea	Ea		MoU		Ę,	r A	EA	A3	EA CA	TA A	EA	EA	EА	ΕA	ĒA	1	EA	2 5	V.3	- Karrs
6	1	2		5	4	2000	2000		0 0	, 1	1	□		γτρ			2	6	+	۱,	; -	 	12	-	12	12		1000	-	. 8	
	YY-800	F-210 PRO	100027 100017 100071		M80 with 12 lead ECG		SE-1200	027041-4	CVUOA1 A	HD-7	FRED PA-1	YX-280D 18L		MODE/CAT No		1-710 PRO	SKB041-3S	Gradian CCV	OCA-10 DOD FLOW	1-100	HD-7	SE-1200	AIP-1200	i15	iM70 with mobile trolley	D8D			0071-35	1	
FAZZINI	SYSMEDICAL	FAZZINI		FAZZINI	FDAN	achiero	EDAN	SAIKANG	FAZZINI	SCHILLER	SCHILLER	ARI MEDICAL TECHNLOGIES	ITX.	BRAND/MANUFACTUR		FAZZINI	SAIKANG	GRADIAN HEALTH	3AITO-22	FAZZINI	SCHILLER	EDAN	ARI MEDICAL TECHNOLOGIES	EDAN	EDAN	SAIKANG		SCHILLER	EDAN	SCHILLER	200000
70,000.00	6,000,000.00	600,000.00		1,800,000.00	9 000 000 00	130.00	5,875,000.00	100,000.00	10,000.00	22,500,000.00	3,500,000.00	910,000.00		Unt Price		600,000.00	2,500,000.00	28,000,000,00	5,000,000.00	2,800,000.00	22,500,000,00	5,875,000.00	1,900,000.00	19,000,000.00	5,000,000.00	6,750,000.00		130,00	5,875,000.00	450,000.00	
420,000.00	6,000,000,00	1,200,000.00		00.000,000.6	600,000.00	260,000,00	5,875,000.00	800,000,00	60,000.00	22,500,000.00	3,500,000.00	910,000.00		Line Total	,	1,200,000.00	5,000,000.00	168,000,000.00	20,000,000.00	33,600,000.00	22,500,000.00	5,875,000.00	22,800,000.00	19,000,000.00	60,000,000.00	81 000 000 00		130,000.00	5,875,000.00	9,000,000.00	

197		195	194												188		186	185	184	183	787	107	180	179			178	1/				176					1/4
63	19	60	20	2	1 6	41	40							35		27	26	25	24	6	v	1 2	× ω	1	ICU		82	δ							75	73	21
Voltage stabiliser	Ultrasound probe covers with (abdominal,linear and cardiac probe)	Portable Ultrasound machine	Suction device: powered (electric or pneumatic)	outtion device: manual (bulb) or toot pump	otretchers and gurneys (wheeled stretchers)	Nebulizer machine	Nebulization masks with tubing (pediatric and adult sizes) (child/adult)	+ 100065 FIBER-OPTIC HANDLE FOR CHILD	W\3 S.S.BLADES SIZE 00,0,1 W/CARRYING CASE 97.60	100071 FIBER-OPTIC MILLER LARYNGOSCOPE COMPLETE MATT TYPE	+ 100017: LARYNGOSCOPE HANDLE FOR ADULT MATT TYPE	S.S. BLADES SIZE 0,1,2,3, and 2 spare bulbs, W/CARRYING CASE	100027 McINYOSH LARYNGOSCOPE COMPLETE MATT TYPE WA	Larynposcone set frange of blades and stock	ECG leads stickers/electrodes	ECG paper	ECG machine with 12 lead electrodes	Drip Stand	Defibrilator with pacing capabilities	Autoclave (electric or non-electric) and supplies	ABG machine with reangent	ividiciparameter cardiac monitor	Portable mechanical ventrator-infant- adult	ICU Beds with CPR capability			X-ray viewing box or digital system	Ultrasound machine with abdominal linear and cardiac probe	SET OF 5 NEOPRENE SPLINT W/CARRYING BAG	NEOPRENE SPLINT FOR FOREARM	NEOPRENE SPLINT FOR ELBOW / ANKLE	NEOPRENE SPLINT FOR LEG	NEOPRENE SPLINT FOR ARM	NEOPRENE SPLINT FOR WRIST	Tension or traction enliet (a.g. base saliet)	Stretion devices politored falactein as a contract.	The second of th
Ea	Ea	Ea	Ea	Ea	Ea	Ea	50pcs						5	2007	500/p	Roll/100pcs	بر ا	E d	E	Ea	Ea	Ea	Ea	Ea			Еa	Ea						130	63		
ហ	ثر	1	2	4	4	2	20						,	20	20	70	_	20	-	1	1	12	9	12			1	ш						4	~	_	
		ECHO ULTRASOUND)	F-30.65/PF	F-175	SKB041-3S	F-210 PRO	05.5009/05.5010	COUNT	1000/1			100017	100027			LF APOC	SE-1200	SKH041-4	Hn.7	YX-280D 18L	115	iM80 with 12 lead ECG	Gradian CCV	D8D			SK-L516	MyLab Sigma (PORTABLE ECHO ULTRASOUND)	DA-02310	DA-02304	DA-02303	DA-02302	DA-02300	מארח אח	F-30.65/PF	F-1/5	
		ESAOTE	FAZZINI	FAZZINI	SAIKANG	FAZZINI	FAZZINI						FAZZINI	NAME	CONT	EDAN	EDAN C	SAKANG	CCHILLED	ARI MEDICAL TECHNIOGIES	EDAN	EDAN	GRADIAN HEALTH	SAIKANG			SAIKANG	ESAOTE						FAZZINI	FAZZINI	FAZZINI	
1,500,000.00	250,000.00	64,000,000.00	1,800,000.00	570,000.00	2,500,000.00	600,000.00	250,000.00						On non'one'T	85,000,00	50,000,00	טטיסטיסיסים מי	E 87E 000.00	100,000,00	73 500 000 00	910 000 00	19,000,000.00	9,000,000,00	28,000,000,00	6,750,000.00		0.000.00	מבה חסח חם	64,000,000.00						700,000.00	1,800,000.00	570,000.00	
7,500,000.00	250,000.00	64,000,000.00	3,600,000.00	2,280,000.00	10,000,000.00	1,200,000.00	5,000,000.00					3	3,500,000.60	1,300,000.00	00,000,000	2,5/2,000,00	500,000,00	00.000,000	27 500 000	910,000.00	19,000,000.00	108,000,000.00	168,000,000.00	81,000,000,00		000,000,000	00 000 028	64,000,000.00						2.800,000.00	3,500,000.00	1,140,000.00	

222	221	22C	219	217	21/	917	215	214	213			21.2		710		208	207	206	199 200 201 203 205 205	198
41	38	31	30	67	25	20	19	28	8	ICU	00	36	1,	27	;	22	16	15	LOT NO ITEM # EMD 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1	66
Refrigerator with thermometer	Heavy duty stretchers	Nebulizer machine	Nebulization masks with tubing (pediatric and adult sizes) (child/adult)	Heavy duty mechanical ventilator sizes)	Public In-unit communication system	Multi-parameter wall mounted cardiac	Defibrillator pads	Defibrilator with pacing capabilities	Automated external defibrilator (AED)		Ariay viewing dox or digital system	Portable Ultrasound (TVS) probes	Menuital Maculine	Nebulization masks with tubing (pediatric and adult sizes) (child/adult)	A Company between control infalliful	Portable patient cardiac Monitor	Vein Viewers	Portable ECG machine with 12 lead electrodes and stand	LOT No. 6: NJOMBE REGIONAL REFERRAL HOSPITAL ITEM # ITEM Standard ICU Beds 1 Standard ICU Beds 1 Heavy duty mechanical ventilator 3 Multi-parameter wall Mounted cardiac monitors 4 Automated external defibrilator (AED) 12 Defibrilator machine with pacing capability 13 Defibrilator pads 14 Laryngoscope set (range of blades and sizes) 16 Laryngoscope set (range of blades and sizes) 17 Laryngoscope set (range of blades and sizes) 18 Laryngoscope set (range of blades and sizes) 19 Laryngoscope set (range of blades and sizes) 100027 McINTOSH LARYNGOSCOPE COMPLETE MATT TYPE W\A 100017: LARYNGOSCOPE HANDLE FOR ADULT MATT TYPE 100071 FIBER-OPTIC MILLER LARYNGOSCOPE COMPLETE MATT TYPE 100071 FIBER-OPTIC HANDLE FOR CHILD 11 PATCH SEC	X-ray viewing box or dig tal system
Ea	Ea	E3	50pcs	Ea	Ea	Ea	Pairs	Ea	Ea		Ea	Ea	Ea	50pcs	E3		Eа	Еа	UoM Ea	Ea
1	12	4	20	2	1	4	10	1	1		-	1	2	20	7	,	2	1	QTY 25 26 26 26 11 1 1 1 5 5	2
YY-800	SKB041-35	F-210 PRO	05.5009/05.5010	Gradian CCV		iM70 with wall mounting		HD-7	FRED PA-1		SK-L516	ECHO ULTRASOUND)	F-210 PRO	05,5009/05.5010	iM80 with 12 lead ECG		QV-500	SE-1200	MODE/CAT No D8D Gradian CCV iM70 with wall mounting FRED PA-1 HD-7 100027 100071 100065	SK-L516
SYSMEDICAL	SAIKANG	FAZZINI	FAZZINI	GRADIAN HEALTH		EDAN	SCHILLER	SCHILLER	SCHILLER		SAIKANG	ESAOTE	FAZZINI	FAZZINI	EDAN	TECHNOLOGIES	ARI MEDICAL	EDAN	BRAND/MANUFACTUR SAIKANG GRADIAN HEALTH EDAN SCHILLER SCHILLER SCHILLER FAZZINI	SAIKANG
6,000,000,00	2,500,000,00	600,000.00	250,000,00	28,000,000.00		4,900,000.00	450,000.00	22,500,000.00	3,500,000.00		850,000.00	64,000,000.00	600,000.00	250,000.00	9,000,000.00	3,500,000.00		5,875,000.00	Unt Price 6,750,000.00 28,000,000.00 4,900,000.00 3,500,000.00 22,500,000.00 450,000.00 1,800,000.00	850,000.00
6,000,000.00	30,000,000,00	2,400,000.00	5,000,000.00	56,000,000.00		19,600,000,00	4,500,000,00	22,500,000,00	3,500,000.00		850,000.00	64,000,000.00	1,200,000.00	5,000,000.00	18,000,000.00	on'noo'noo'n	7 000 000 00	5.875.000.00	Line Total 175,500,000.00 728,000,000.00 127,400,000.00 3,500,000.00 22,500,000.00 4,500,000.00 9,000,000.00	1,700,000,00

1	247	246	245	1447	243	1	243	240	239	238		ediam.	237	236	725	233		231	230	229	228	227	226					224	223
	20	92	Çe Ce	/4	71	C	a c	59	58	54		52		3 04	2	32	101	28	27	24	23	22	ű	EMD	ITEM#	LOT No.	1	54	52
Microscope	A-ray viewing box of digital system	Wheelchairs	Ultrasound machine with abdominal, cardiac and liner probe	Ketrigerator with thermometer	Patient Wheelchairs	neavy outy Oxygen concertator	Nepolitei Hachine	Nebulization masks with tubing (pediatric and adult sizes) (child/adult)	Nebulization masks with tubing (pediatric and adult sizes) (child/adult)	Portable ventilation(pediatrics-adult capability)	100071 FIBER-OPTIC MILLER LARYNGOSCOPE COMPLETE MATT TYPE W/3 S.S.BLADES SIZE 00,0,1 W/CARRYING CASE 97.60 + 100065 FIBER-OPTIC HANDLE FOR CHILD	S.S.BLADES SIZE 0,1,2,3, and 2 spare bulbs, W/CARRYING CASE + 100017: LARYNGOSCOPE HANDLE FOR ADULT MATT TYPE	100027 McINTOSH (ARVNGOSCOBE COMBIETE MATT TOST OF	Electronic cardiac monitor (mobile)	red dishosable electrodes	ECG paper	ECG machine with 12 leads electrodes	Drip Stand	Fetal Doppler	Defibrilator with pacing capabilities	Defibrilator pads	Delibrilator (with manual controls, syncronizing, and cardioversion capabilities)	Automated external defibrilator (AED)		ITEM	7: Mbeya Regional Referral Hospital	A-ray viewing dox or digital system	Vein viewers (finder)	Portable Ultrasound machine (with abdominal, cardiac and linear)
Each	Each	Each	Each	Each	Each	Each	Each	50pcs	50pcs	Each		en en	Each	Each	Each	Rim	Each	Each	Each	Each	Pairs	Each	Each	0011	1 ion		Еa	Ea	EB
2	4	20	2	3	10	2	ß	20	30	2		u	6	2	5000	20	2	10	10	1	20	1	2	4	QT/		2	2	1
8-292 Pli	SK-L516	9001 STEEL WHEELCHAIR	MyLab Sigma (PORTABLE ECHO ULTRASOUND)	YY-800	9001 STEEL WHEELCHAIR	OLV-10 DUO FLOW	F-210 PRO	05.50090	05.5010	Gradian CCV	100065	100027	im70 with wall mounting	iM70 with trolley			SE-1200	SKH041-4	AFD-640C	HD-7		HD-7	FRED PA-1	MODE/CAL NO	MODE/CAT NO		SK-L516	QV-500	MyLab Sigma (PORTABLE ECHO ULTRASOUND)
OPTIKA	SAIKANG	ARI MEDICAL TECHNOLOGIES	ESAOTE	SYSMEDICAL	ARI MEDICAL TECHNOLOGIES	ZZ-OLIVE	FAZZINI	FAZZINI	FAZZINI	GRADIAN HEALTH		FAZZINI	EDAN	EDAN	SCHILLER	EDAN	FDAN	SAIKANG	ARI MEDICAL	SCHILLER	SCHIII ED	SCHILLER	SCHILLER	BRAND/WANDFACTUR	37		SAIKANG	ARI MEDICAL TECHNOLOGIES	ESAOTE
2,000,000.00	850,000.00	350,000.00	64,000,000.00	6,000,000.00	350,000,00	5,000,000.00	600,000.00	250,000.00	250,000.00	28,000,000.00	Virgin 100 (8)	1,800,000.00	4,900,000,00	5,000,000,00	2,000,00	30,000,00	\$ 875 000.00	100 000 00		22.500.000.00	45,500,000.00	72 500 000	3.500.000.00	Unt Price			850,000.00	3,500,000.00	64,000,000.00
4,000,000.00	3,400,000.00	7,000,000.00	128,000,000.00	18,000,000.00	3,500,000.00	10,000,000,00	3,000,000,00	5,000,000.00	5,000,000.00	56,000,000.00		9,000,000,00	29,400,000.00	10,000,000,00	10 000 000 00	00.000,009	11 750 000 00	1 000 000 00	3,000,000.00	22 500 000 00		22,500,000.00	7,000,000,00	Line Total			1,700,000,00	7,000,000.00	64,000,000.00

1/7	0/7	202	260	320	267	286		264		Γ	263		202	202	263	703			202				261	260	259	258	257	256	255	П	254	253	252	167	250	249
Ig	9	0	0 0	מַ נ	3	46		42			39	Ī	30	3 0	00	3						27	26	25	24	4	w	2	1	Ĉ	TO3	70Z	101	99	98	97
Suction device; powered (electric or pneumatic)	Suction device: manual (bulb) or foot pump	meavy outry stretchers and gurneys (wheeled stretchers)	piculoscope	Total California	Builes ovineer machine with tubing	Nebulization masks with tubing (pediatric and adult sizes) (child/adult)	ABS+steel bedside table, ON 4 WEHEELS	Mobile storage furniture (e.g. trolley)	100071 FIBER-OPTIC MILLER LARYNGOSCOPE COMPLETE MATT TYPE VX\3 S.S. BLADES SIZE 00,0,1 W/CARRYING CASE 97.60 + 100065 FIBER-OPTIC HANDLE FOR CHILD	+ 100017: LARYNGOSCOPE HANDLE FOR ADULT MATT TYPE	100027 McINTOSH LARYNGOSCOPE COMPLETE MATT TYPE WA	Laryngoscope set (range of blades and sizes)	tiectronic multi-parameter cardiac monitor	icco paper, leads electrodes stickers	ECG machine with 12 lead electrodes	Ambu AuraGain Size 6	Ambu AuraGain Size 5	Ambu AuraGain Size 4	Ambu AuraGain Size 3	Ambu AuraGain Size 2%	Ambu AuraGain Size 2	Dual-tube laryngeal mask airway (LMA) (#2 - 7)	Drip Stand	Digital thermometer (32 - 43 Celsius)	Defibrilator with pacing capabilities	Arterial blood gas (ABG) machine	Heavy duty Mechanical Ventilator	Portable mechanical ventilators	ICU Beds with CPR capabilities		Operating Lamp	Dead body stretcher (covered)	Hot air oven	Mobile digital x ray	Examination bed (SK-B1 Examination table)	Centrifuge
EACH	EACH	EACH	EACH	EACH	EACH			EACH				Ea	EACH	EACH	EACH			_				SET/6	EACH	EACH	EACH	EACH	EACH	EACH	EACH		Each	Each	Each	Each	Each	Each
4	2	2	4	5	20	50		S)				UI	12	5000	4		Ī			Ī		20	4	2	2	-	»	4	5		2	2	1	Ľ	4	-
F-30.65/PF	F-175	SKB041-3S		BT710	JF-210 PRO	05.5009/05.5010		SKS013-1	100071 100065	100027			iM80 with 12 lead ECG		SE-1200	408600000	408500000	408400000	408300000	408250000	408200000		SKH041-4		HD-7	115	Gradian CCV	Gradian CCV	DRD		AML700/700 LED	FPMT-006	FN 055	MDR	X09	NF-200
FAZZINI	FAZZINI	SAIKANG	FAZZINI	BISTOS	FAZZINI	FAZZINI		SAIKANG				FAZZINI	EDAN	EDAN	EDAN	<u> </u>	<u> </u>	91	<u> </u>	91		AMBII	CAINANIC	FAZZINI	COMILED	GRADIAN MEALIN	GRADIAN DEALTH	GRADIANI MEAITH	CAIVANG	TECHNOLOGIES	ARI MEDICAL	SYSMEDICAL	NUVE	DEL MEDICAL	SAIKANG	NLIVE
1,800,000.00	570,000,00	2,500,000.00	70,000.00	950,000.00	600,000.00	250,000,00	*10,000,00	450 000 00				1,800,000 00	9,000,000,00	2,000,00	5,875,000.00						*20,000,00	150,000,00	100,000,00	10,000,00	00.000,003 CE	30.000,000,82	20,000,000,00	30,730,000.00	6 450 000		20,000,000,00	uc 000 005 6	uc 000 006 c	OC.000.000.062	00.000.055	חר מתח ממפ כ
7,200,000.00	1,140,000.00	5,000,000.00	280,000.00	4,750,000,00	12,000,000.00	5,000,000.00	4,700,000,00	7700 000				9,000,000.00	108,000,000.00	10.000.000.00	23,500,000,00						9,000,000,00	3,000,000	50,000,00	45,000,000,00	19,000,000	224,000,000.00	00:000,000,211	00.000,000			40 000,000 00	19,000,000	1 000 000 E	200,000,000	20000000	3 000 000 00

297	067	206	7	294	293	292	291	290		289		288	280	700	285	284			283		282	281	280	617	278	2//	276					275	274	2/3
28		20	3	25	24	22	21		8		19	17	; =	:	10	9			CO		17	6	Ų,	+	. ω	2	-	EMD	ITEM#	LOT No	+	69	68	94
CARDIAC TABLE	GEODICE LOCKERS	OPERATING LAMP	COLUMN TO THE PARTY OF THE PART	AUTOCIAVE MACHINE	BLOOD BANK REFRGERATOR	X-RAY VIEWER	DIGITAL MOBILE X-RAY	"SKM-B Mayo trolley	with the Size J	(SKM-B Treatment trolley - Two stainless steel Shelves and one drawer	INSTRUMENT TROLLEY	DEFILERILLATOR MACHINE	INFUSION PUMP		BLOOD AND FLUID WARMER	NEBULIZER MACHINE	100071 FIBER-OPTIC MILLER LARYNGOSCOPE COMPLETE MATT TYPE WAS S.S.BLADES SIZE 00,0,1 W/CARRYING CASE 97.60 + 100065 FIBER-OPTIC HANDLE FOR CHILD	100017: LARYNGOSCOPE HANDLE FOR ADULT MATT TYPE	S.S. BLADES SIZE 0.1.2.3. and 3 spare builts (W/CARBYING CASE)	Laryngoscope set (range of blades and sizes)	HEAVY DUTY SUNCTION MACHINE	BLOOD GAS ANALYSER	PORTABLE ULTRASOUND	PUNTABLE ECG MACHINE	PATIENT MULTIPARAMETER CARDIAC MONITOR	HEAVY DUTY MECHANICAL VENTILATOR	HOSPITAL BEDS		HEM	LOT No. 8: ringa Regional Referral Hospital		X-ray viewing box or digital system	Wheelchairs	Ultrasound probe covers
EACH	EACH	EACH	EACH	DACE.	מיסר ב	FACH	EACH	EACH		EALH	EACH	EACH	EACH	5	פאכם	EACH				£3	EACH	EACH	EACH	EACH	EACH	EACH	EACH	- CONT	Model			EACH	EACH	EACH
J	10	j ⊷	L	-		5	1	Ь		Į.	\$ ~	4	Δ	,		,				5	w,	-	1	1	5	2	10	4	OT V			US C	ו ת	2
SKHOAZ	SKSOCZ	ALM700/700 LED	NC 32	BBR-4V1000	מזיינטנט	CV 1616	MOR	SKH038-2		SKHOOI	HD-7	ASP-1500	AIP-1200	POTENT	15-210 PRO		100071	100017	100027		f-100	ECHO OLI NASCONDI	MyLab Sigma (PORTABLE	SE-1200	iM80 with 12 lead ECG	Gradian CCV	A1K	WICDE/CAL NO	MODE CAT NO			SK-1516	מחחל כדבבו אושבבו בשאים	
CARANT	SAIKANG	TECHNOLOGIES	NUVE	BIOBASE	DAIKANG	DECMIEDICAL	Din Andron	SAIKANG		SAIKANG	SCHILLER	TECHNOLOGIES	ARI MEDICAL TECHNOLOGIES	B(O·X	FAZZINI					FAZZINI	EAZZINI	EDANI		EDAN	EDAN	GRADIAN HEALTH	SONANIAS	BRAND/MANUFACTUR			GRIPS AG	SAINANG SAN MAN SAN SAN SAN SAN SAN SAN SAN SAN SAN S		
100,000.00	200,000,00	20,000,000.00	19,000,000.00	19,000,000.00	850,000.00	00,000,000,062		300,000.00		500,000.00	22,500,000,00	2,000,000.00	1,900,000,00	5,000,000.00	600,000.00				1,000,000.00	1 800 000 00	00,000,000,61	64,000,000 00		5,875,000,00	00,000,000,00	78 000 000 00	900 000 00	Unt Price			00.000.058	350,000 00	250,000.00	0.0000000000000000000000000000000000000
20,000,000,00	2,000 000 00	20,000,000.00	19,000,000.00	19,000,000.00	8,500,000,00	290,000,000.00		1,500,000.00		5,000,000.00	45,000,000.00	8,000,000.00	7,600,000,00	10,000,000 00	3,000,000,00				2,000,000,00	8,400,000.00	19,000,000.00	a designation of	64,000,000,00	5 875 000 00	13.000,000,00	56 000 000,00		Line Total			4,250,000 00	2,100,000.00	500,000,00	00.000,000.00

				İ	Ì			ſ
0						INSTALLATION, TRAINING, TESTING AND COMMISSIONING CHARGES INCLUDED	323	
48,000,000.00	6,000,000,00	00	PER SITE/DESTINATION			TRANSPORT TO RESPECTIVE DESTINATIONS AS PER TENDER DISTRIBUTION LIST	322	
21,585,511,000.00		SUB TOTALTOTAL	ΠS					
1,500,000.00	1,500,000.00	SAIKANG	SKR054-ET	1	EACH	RESUSCITATION TROLLEY WITH CPR BOARD SKM-B Emergency trolley	321 28	ω
65,000.00	130.00			500	EACH		320 26	ω
55,000,000.00	55,000,000.00	UTAS	U-VENT	1	EACH			w
2,400,000.00	200,000.00	SAIKANG	SKS002	12	EACH	BEDSIDE LOCKERS	318 22	w
50,000.00	25,000.00	ALLMEDICUS	GLUCO-DR AUTO (AG4000)	2	EACH	GLUCOMETER	317 11	w
1,700,000.00	850,000.00	SAIKANG	SK-L516	2	EACH	X-RAY VIEWER	316 20	w
290,000,000.00	290,000,000.00	DEL MEDICAL	MDR	1	EACH			W
2,850,000.00	950,000.00	S015IB	BT710	3	EACH	PORTABLE PULSE OXIMETER		w
90.000,000,8	2,000,000.00	ARI MEDICAL TECHNOLOGIES	ASP-1500	4	EACH	SYRINGE PUMP	313 12	w
11,400,000.00	1,900,000.00	ARI MEDICAL TECHNOLOGIES	AIP-1200	6	EACH	INFUSION PUMP	312 11	w
2,400,000.00	600,000.00	FAZZINI	F-210 PRO	4	EACH	NEBULIZER MACHINE	311 9	L
			100017 100071 100065			S.S.BLADES SIZE 0,1,2,3, and 2 spare bulbs, W/CARRYING CASE + 100017: LARYINGOSCOPE HANDLE FOR ADULT MATT TYPE 100071 FIBER-OPTIC MILLER LARYINGOSCOPE COMPLETE MATT TYPE W\3 S.S.BLADES SIZE 00,0,1 W/CARRYING CASE 97.60 + 100065 FIBER-OPTIC HANDLE FOR CHILD	CO	S
3,600,000.00	1,800,000.00	FAZZINI	100037	2	Ea	Laryngoscope set (range of biades and sizes) 100027 McINTOSH LARYNGOSCOPF COMPLETE MATT TYPE WA	010	CA.
8,400,000.00	2,800,000.00	FAZZINI	F-100	3	EACH	HEAVY DUTY SUNCTION MACHINE	L	w
38,000,000.00	19,000,000.00	EDAN	115	2	EACH	BLOOD GAS ANALYSER	308 6	w
64,000,000.00	64,000,000.00	ESAOTE	MyLab Sigma (PORTABLE ECHO ULTRASOUND)	1	EACH	PORTABLE ULTRASOUND MACHINE	307 5	ω
5,875,000.00	5,875,000.00	EDAN	SE-1200	ы	EACH	PORTABLE ECG MACHINE	306 4	w
58,800,000,00	4,900,000,00	EDAN	iM70 with wall mounting	12	EACH	PATIENT MULTI-PARAMETER CARDIAC MONITOR	305 3	w
25 000 000 00	78 000 000 00	GRADIAN HEALTH	GRADIAN CCV	2	EACH	HEAVY DUTY MECHANICAL VENTILATOR	304 2	ω,
81 (20 000 00	מ שבת מתח מת	CAIKANIG	חאח	13	FACH	STANDARD ICU BEDS	303 1	ω
550,000,00	550,000.00	FAZZINI		1	EACH	WALL MOUNTED OPTHALMOSCOPE	SUZ 35	Ų.
58 000 000 00	58,000,000.00	GRADIAN HEALTH	UAM	J-3	EACH			Ų.
15 000 000 00	15,000,000.00	SAIKANG	A301	Ļ	EACH			Ψ
55,000,000.00	55,000,000.00	UTAS	U-VENT	→	EACH	NEGNATAL VENTILATOR		2
6,800,000.00	3,400,000.00	ARI MEDICAL TECHNOLOGIES	AFM-800	2	EACH	FOETAL MONITOR	298 29	12
								1

Delivery Terms DDP to AS PER TENDER DELIVERY SCHEDULE KAS MEDICS LTD.

Bid Validity Period 120 days

DAR-ES-SALAM

Authorized Signatory CHARLES LINTU in the Capacity of SALES ADMINISTRATIVE EXECUTIVE SIGNED FOR: KAS MEDICS LIMITED Date: 25th November 2021 PAYMENT SCHEDULE DESCRIPTION
Advance payment, after contract signing After Delivery P.O. Box 7856 Dar as Sulasm Tanzahia, Tel +255 22 2861737/4. Breatl info@kasmedics.com, PERCENTAGE 21,633,511,000,00

KAS MEDICS LIMITED

Your partner in progressive healthcare



Date: 24th November, 2021.

To:
Secretary,
MZRH Tender Board,
P. O. Box 419,
Mbeya,
Tanzania.

THAT BY THIS POWER OF ATTORNEY given on the 24th November, 2021.

WE the undersigned KAS MEDICS LIMITED of Vingungti Industrial Area, Plot No. 11, Umoja Complex Warehouse, 1st Floor, UF09&10, by virtue of authority conferred to us, do hereby ordain nominate and appoint CHARLES LINTU of P. O. Box 7856 Dar Es Salaam, to be our true lawful Attorney and Agent, with full power and authority, for us and in our names, and for our accounts and benefits, to do any, or all of the following acts, in the execution Tender No. ME/007/MBY/2021/22/CS/MV/09 is to say; To act for the company and do any other thing or things incidental for Tender No ME/007/MBY/2021/22/CS/MV/09 of SUPPLY, INSTALLATION, TESTING, COMMISSIONING AND TRAINING OF MEDICAL EQUIPMENT.

AND provided always that this Power of Attorney shall not revoke or in any manner affect any future power of attorney given to any other person or persons for such other power or powers shall remain and be of the same force and affect as if this deed has not been executed.

AND we hereby undertake to ratify everything, which our Attorney or any substitute or substitutes or agent or agents appointed by him under this power on his behalf herein before contained shall do or purport to do in virtue of this Power of Attorney.

SEALED with the common seal of the said KAS MEDICS LIMITED and delivered in the presence of us this 24th day of November, 2021.

IN WITNESS whereof we have signed this deed on this 24th day of November, 2021 at Vingungti Industrial Area, Plot No. 11, Umoja Complex Warehouse, 1st Floor, UF09&10 for and on behalf of KAS MEDICS LIMITED

SEALED and DELIVERED by the Common Seal of KAS MEDICS LIMITED This 24th day of November, 2021.

COMMISSIONER FOR OATHS

DONOR (signature)

KAS MEDICS LTD. P. O. Box 7856 DAR-ES-SALAAM TANZANIA

www.kasmedics.com

KAS MEDICS LIMITED

Your partner in progressive healthcare



Tender Securing Declaration

Date: 24th November, 2021.

Tender No: ME/007/MBY/2021/22/C5/MV/09.

To: Secretary, MZRH Tender Board, P. O. Box 419, Mbeya, Tanzania.

We, the undersigned, declare that:

We understand that, according to your conditions, tenders must be supported by a Tender Securing Declaration.

We accept that we will be automatically suspended from being eligible for tendering in any contract with the Purchaser for the period of two years started from date of bid opening, if we are in breach of our obligation(s) under the tender conditions, because we:

- (a) Have withdrawn or modified our Tender during the period of tender validity specified in the Form of Tender.
- (b) Disagreement to arithmetical correction made to the tender price; or
- (c) Having been notified of the acceptance of our Tender by the Procuring Entity during the period of tender validity, (i) failure to sign the contract if required by Procuring Entity to do so or (ii) fail or refuse to furnish the Performance Security, or to comply with any other condition precedent to signing the contract specified in the tendering documents.

We understand this Tender Securing Declaration shall expire if we are not the successful Tender, upon the earlier of (I) our receipt of your notification to us of the name of the successful Tender; or (ii) twenty-eight (28) days after the expiration of our Tender.

RAS MEDICS LTD.

Signed:

P.O.Box 7856 DAR-ES-SALAAM

TANZANIA

Name: Charles Lintu in the Capacity of Sales Administrative Executive

Duly authorized to sign the Tender for and on behalf of Kas Medics Limited

Dated 24th day of November 1977

Attested by me:

Advocate

THE UNITED REPUBLIC OF TANZANIA



MINISTRY OF HEALTH, COMMUNITY DEVELOPMENT, GENDER, ELDERLY AND CHILDREN

Cable referral hospital

Telephone: 2503456/2503351

Fax: 2503577



MBEYA ZONAL REFERRAL HOSPITAL P.O.BOX 419

MBEYA

Please quite:

Ref. No. MZRH/AD.121/345/02/F.

23rd December 2021

Kas Medics Limited,

P.O.BOX 7856.

Dar Es Salaam.

RE: NOTIFICATION OF AWARD FOR CONTRACT NO. ME/007/MBY/2021-2022/G/1. FOR SUPPLY,INSTALLATION,TESTING,COMMISSIONING AND TRAINING OF MEDICAL EQUIPMENT

Reference is made to the above heading.

This is to inform you that you have been awarded Tender dated 26th November 2021 for execution of the Supply, Installation, Testing, Commissioning and Training Of Medical Equipment Tender No. ME/007/MBY/2021-2022/G/1 The bid price is 182,748,000/= Tanzanian shillings for Iringa RRH, 438,230,000/= Tanzanian shillings for Mbeya RRH, 347,262,000/= Tanzanian shillings For Mbeya ZRH, 231,292,500/= Tanzanian shillings for Njombe RRH, 403,296,000/= Tanzanian shillings for Songea RRH, 388,936,000/= Tsh For Songwe RRH and 450,865,000/= Tanzanian shillings For Sumbawanga RRH,

You are therefore required to confirm your acceptance in writing to the undersigned immediately for further action

Your Sincerely,

Executive Director Mbeya Zonal Referral [1995]

Dr. Mbwanji, G.F

May Till, is

EXECUTIVE DIRECTOR

MUHTASARI WA MAJADILIANO NA MARIDHIANO BAINA YA HOSPITAL ZA RUFAA ZA KANDA NA HOSPTALI ZA RUFAA ZA MIKOA YA NYANDA ZA JUU KUSINI PAMOJA NA WAZABUNI WA VIFAA NA VIFAA TIBA TAREHE 02.12.2021

AGENDA

- 1. Kufungua Kikao
- 2. Vigezo vinavyotumika katika majadiliano na maridhiano
- 3. Majadiliano na Wazabuni
- 4. Mengineyo
- 5. Kufunga kikao

MAUDHURIO:

NA		СНЕО	ANAPOTOKA	NAMBA YA SIMU
1	Dr Raphael Gabriel	Mwenyekiti	MZRH	0763125448
2	Dr Mdede Musa L	Mjumbe	MZRH	0765815179
3	Kelvin Warioba Makoba	Mjumbe	RSO	0743114247
4	Salum Ng'onze	Mjumbe	SONGWE-RRH	0769006082
5	Ritha E Mlay	Mjumbe	MZRH	0756604601
6	Eonike Wavenza	Mjumbe	MZRH	0754542497
7	Elias N Mshana	Mjumbe	MZRH	0763016150
88	Julieth Rogastian Laswai	Mjumbe	MZRH	0718876950
9	Petro Peter Songi	Mjumbe	MBEYA-RRH	0718362333
10	Ditram Mendruf Mbunza	Mjumbe	MBEYA-RRH	0/5404/526
11	Aloyce Kavumika	Mjumbe	NJOMBE-RRH	0713894483
12	Shomari Omari Masenga	Mjumbe	NJOMBE-RRH	0758586032
13	Scholastica Laurent	Mjumbe	IRINGA-RRH	0755780918
14	Edgar Gabone	Mjumbe	IRINGA-RRH	0621009010
15	Obedi Daniel	Mjumbe	SONGWE-RRH	0782279398
16	Dr Salma M Bajber	Mjumbe	SONGWE-RRH	0684378815
17	Lusekelo Mwakatobe	Mjumbe	MZRH	0714441971
18	Sunday G Kanyama	Mjumbe	SONGEA-RRH	0764776470
19	Cecilia Ngatunga	Mjumbe	MZRH	0713644195
20	Haika Maro	Mjumbe	MZRH	0738656552
21_	Angelica Wavenza	Mjumbe	RAS	0754542547
22	Ambele Philip	Mjumbe	S/WANGA-RRH	0784487150
23	Prosper Massawe	Mjumbe	S/WANGA-RRH	O759735903
24	Naima Mkingule	Mjumbe	MZRH	0715678888
25	Alinanuswe Mwansasu	Katibu	MZRH	0765314230

I. KUFUNGUA KIKAO

Mwenyekiti alifungua kikao mnamo saa 05:51 Asubuhi kwa MAOMBI, na kuwakaribisha wajumbe katika kikao. Mwenyekiti alieleza kwenye kikao kuwa tunawawakilishi kutoka Ofisi ya Usalama Mkoa (RSO), Ofisi ya Katibu Tawala Mikoa (RAS), Hospitali za Mikoa ya Iringa, Njombe, Mbeya, Songwe, Songea, Sumbawanga na wenyeji kutoka Hospitali ya Rufaa ya Kanda Mbeya pamoja na wazabuni wa makampuni sita ikiwa ni Mokasi Medical System, Pacific, Fabstech, Computertech, Anudha Ltd na Kas Medics Ltd.

Baada ya utambulisho huo mwenyekiti alitoa fursa kwa kila Mjumbe aweze kujitambulisha kwa jina na eneo analotoka. Wajumbe wa kikao walijitambulisha.

2. VIGEZO VINAVYOTUMIKA KATIKA MAJADILIANO NA MARIDHIANO:

Mwenyekiti alieleza kwenye kikao kuwa, kutakuwa na mjumbe ambaye atatupitisha na kutolea ufafanuzi katika kuongoza kikao na kufahamu vigenzo vitakavyotumika, Mwenyekiti alimkaribisha mjumbe aweze kueleza lengo na vigezo vitakavyotumika.

Mjumbe alijitambulisha na kuelezea vigezo vitakavyotumika katika majadiliano na maridhiano baina ya wajumbe kutoka katika Hospitali za Rufaa za Mikoa na Kanda na wazabuni wa makampuni yote yaliyoomba tenda ya kuuza na kusambaza vifaa na vifaa tiba.

Mjumbe alieleza vigezo hivyo kama ifuatavyo:-

- Gharama ya vifaa tiba, lengo ni kuangalia gharama nafuu bila kuathiri ubora uliopendekezwa. Pia kuzingatia gharama ambazo wamenukuu kama zina kodi ndani yake.
- ii. Huduma zitakazotolewa ikiwa na aina ya mkataba utakaotumika baada ya kupatiwa huduma kama utahusisha matengenezo bila gharama ya vifaa na ujira au ujira pekec yake, Pia wanakuwa na mwitikio kiasi gani kifaa au mtambo utakapopata shida au kuharibika (muda wa matengenezo). uwepo wa wahandisi vifaa tiba na watalamu wanaohusika na matengenezo (Idadi ya wataalamu walionao) na ujuzi wao,
- iii. Kupokea na kusimika vifaa na vifaa tiba/ mitambo, ilielezwa kuwa ni lazima tufahamu kuwa baada ya kushinda zabuni tujue vifaa vitaweza kupokelewa na kusimikwa kabla ya mwezi Aprili 2022.

- iv. Utaratibu wa malipo, ulielezwa kuwa ni łazima tuzingatie namna ambayo watatakiwa kulipwa kwa sababu fedha zitakuwa zinaletwa kwa awamu.
- V. Upatikanaji wa spea na vifaa vinavyotumika katika mashine mbalimbali, ilielezwa kuwa kama mzabuni atashinda zabuni ni lazima tufahamu kama vifaa vya mashine/mtambo vitahitajika, je? vinapatikana kwa urahisi ikiwa vipo nchini au kuagizwa na kama vinaagizwa nje ya nchi wanatuhakikishia vitachukua muda gani hadi kufika.

Baada ya mjumbe kutoa vigezo vitakavyotumika aliwasilisha kwenye kikao.

Mwenyekiti aliwakaribisha wajumbe kwa ajili ya kuchangia kama kuna la ziada katika vigezo hivyo.

Wajumbe wa kikao waliridhia vigezo hivyo na kushauri kuwa ni vema katika upande wa gharama ukidhi bajeti za hosptali zilizotengwa bila kuathiri ubora wa vifaa na vifaa tiba/mitambo vitakavyonunuliwa, pia tuangalie na uwezo wa mzabuni katika kuuza na kusambaza vifaa tiba kwa wakati kutokana na muda uliopangwa.

Mwenyekiti aliwashukuru wajumbe kwa michango yao pia alisisitiza kila hospitali kuangalia bajeti yake iliyotengwa kwa ajili ya ununuzi wa vifaa, vifaa tiba, mitambo na ujenzi ili esiashiri zoezi zima.

3. MAJADILIANO NA WAZABUNI:

Mwenyekiti aliwakaribisha wazabuni wote na kuwashukuru kwa mwitikio wa kuweza kufika, pia aliwatambulisha wajumbe na kuwaeleza kuwa wajumbe waliopo kuna uwakilishi kutoka Hospitali sita za Rufaa za mikoa ya Iringa, Njombe. Mbeya, Songea, Songwe na Sumbawanga na wenyeji wao Hospitali ya Rufaa ya kanda Mbeya, na kuna wageni kutoka Ofisi ya Usalama Mkoa (RSO) na Ofisi ya Katibu Tawala Mkoa (RAS) pamoja na wazabuni wa makampuni sita ambayo ni Mokasi Medical System, Pacific, Fabstech, Computech Anudha na Kas Medics Ltd.

Mwenyekiti baada ya kutoa utambulisho huo alimkaribisha mjumbe aweze kutoa utaratibu utakaotumika katika kuongoza majadiliano na maridhiano ya zabuni wafizoomba.

Mjumbe alieleza kwenye kikao vigezo na utaratibu utakaotumika katika majadiliano na maridhiano kama vilivyoainishwa katika agenda namba 2.

Mwenyekiti aliwakaribisha wazabuni na kuanza majadiliano kwa kila mzabuni kama zifuatavyo;-

I. MOKASI MEDICAL SYSTEM:

Mzabuni kutoka kampuni ya Mokasi alimshukuru mwenyekiti na wajumbe na kueleza kwenye kikao gharama za vifaa na vifaa tiba kama alivyonukuu kwenye zabuni.

a. MTAMBO WA CT - SCAN:

Mzabuni alieleza kwenye kikao kuwa gharama ya mtambo mmoja ni Tshs 2,177,280,000/= ikiwa ni seti nzima ambayo inahusu vitu vinavyohusiana na mtambo na visivyohusiana kama ilivyoonesha kwenye zabuni Na. ME/007/MBY/2021-2022/G/1 na gharama hizo zinahusisha.

- Mtambo hadi kusimikwa kwenye eneo husika "Delivery to site"
- Mkataba wa matengenezo kwa miaka mitano" warranty" (comprehensive)
- Mafunzo kwa watumiaji na mafundi.
- Kuwepo na wataalamu katika kanda zote kwa ajili ya matengenezo na marekebisho ya kifaa/ mtambo ukipata shida au kuharibika.
- Gharama hizo hazina kodi ndani yake kwa sababu serikafi ilitoa msamaha katika uagizaji wa vifaa na vifaa tiba kwa ajili ya matumizi ya hospitali.

Baada ya mzabuni kuelezea hivyo aliomba apate muongozo wa kujua kama kuna kitu kimesahaulika au atoe maelezo sehemu ambazo hazijaeleweka.

Mwenyekiti alishukuru na kuwakaribisha wajumbe kwa majadiliano:

Wajumbe wa kikao walipenda kufahamu kuwa endapo atashinda zabuni utaratibu wa malipo upoje, pia waliomba gharama iweze kushuka kwa kuwa fedha iliyotengwa katika bajeti haikidhi gharama hizo kwa maelezo kuwa fedha iliyotengwa inahusisha ununuzi wa mtambo /machine ya CT Scan pamoja na ujenzi wa jingo au maboresho kwa maeneo ambayo yanajengo. Aidha upunguzwaji wa gharama hizo usiathiri ubora wa kile walichokiomba.

Mzabuni alieleza kuwa kwa upande wa namna ya kulipa wao hawana tatizo watasikiliza wateja wanataka malipo yaweje pia alipenda kufahamu malipo yanafanywa na Serikali Kuu/Hospitali husika, hivyo kama watapewa muongozo wa namna ya kulipa hakuna tatizo ila kuwepo na "Guarantee letter of payment" "letter of credit".

Wajumbe wa kikao waliomba gharama hiyo iweze kupungua uendane na uhalisia wa bajeti zao na wakapenda kufahamu endapo baadhi ya vitu vikapungua kama warrant itapungua ibakie kwa mwaka mmoja na labour miaka mine.

Mzabuni alieleza kwenye kikao kuwa gharama ya matengenezo inaweza kupungua kwa kiasi cha USD 1600 kwa rate ya 2340 kwa miaka minne ambayo ni sawa na Tsh 37,40,000/= hivyo na kufikia jumla ya Tsh 512, 560,000/=

b. MTAMBO WA CT - SCAN:

Mzabuni alieleza kwenye kikao kuwa gharama aliyoiweka ilikuwa hajahusisha upande wa vifaa ambavyo ni "non Ct Scan component" na kufanya kiasi cha Tsh 2,098,980,000/= na ikiwa na vifaa hivyo inakuwa jumla ya Tsh 2, 189,000,000/= gharama hizo zinahusisha:

- Kufikisha na kusimika mtambo
- Matengenezo miaka mitano (comprehensive)
- Mafunzo kwa watoa huduma
- Wataalamu na vifaa kuwopo pale vinapohitajika
- Mzabuni alishauri wajumbe kwa vitu ambayo ni "non- medical component" vitolewe kwa kuwa vinaongeza gharama na sio sehemu ya mashine ya CT- Scan.

Wajumbe wa kikao walitushukuru kwa ushauri na kuomba aweze kupunguza gharama ili tuendane na bajeti ya ununuzi na ujenzi wa majengo ya kusimika vifaa hivyo.

Mzabuni alieleza kwenye kikao kuwa gharama ambazo atapunguza ni uhalisia awezi kushuka zaidi ya hapo na kusema kuwa gharama ikiwa na vifaa vyote vya CT - Sean na "non CT -Sean component" ni Tshs 2,189,000,000/= na vifaa visivyokuwa na "non CT -Sean component" ni Tshs 2,090,000,000/=.

Pia alieleza utaratibu wa malipo ni malipo ya namna tatu, malipo ya awali (Advance paymen) ya asilimia 60%, "Delivery of machine" asilimia 30% na 10% "after installation", "commission" na kwa mafunzo malipo yatafanyika kwa "letter of credit" kwa kila awamu (Phase).

III. FABSTECH:

Mzabuni alijitambulisha na kueleza kuwa yeye anahusika na upande wa ufungaji wa mfumo katika Hospitali "Felemedicine".

Hivyo kutokana na zabuni aliyokuwa amepewa kuna kifaa kimoja kimebadilishwa na kufanya gharama kuongezeka kutoka Tshs 6,000,000 na kufikia Tshs 24,000,000 na kufanya gharama kupanda na kufikia Tshs.168,092,533 badala Tsh 150,381,933 iliyokuwa ya awali.

Wajumbe wa kikao waliomba kupunguziwa gharama kwa kuwa gharama hizo zipo nje ya bajeti za taasisi zao.

Hata hivyo, Mzabuni alieleza kwenye kikao kuwa gharama haiwezi kushuka kwa kuwa hiyo ni gharama halisi ya vifaa na upande wa usafirishaji umekuwa mgumu kwa kuwa upande wa meli inatumia muda mrefu na inabidi watumie usafiri wa anga ili kufikisha kwa wakati pia alishauri kama eneo la kupunguza gharama ni upande wa ufundi ambao badala ya kuwatumia wao, inawezekana kutumia wataalam wa ndani kufunga ambayo ni asilimia 3% ndio inatozwa

Wajumbe walipenda kujiridhisha ubora na uimara wa vifaa hivyo.

Mzabuni alieleza kuwa vifaa vingi vya TEHAMA vinakuwa na bora na pia ikitokea kinashida uwezekano wa kubadilishwa unakuwepo na upatikanaji wake ni iahisi.

IV. COMPTECH (GE)

a. MTAMBO WA DIGITAL X- RAY - MACHINE

Mzabuni alieleza kwenye kikao kuwa gharama za mashine ya Digital X-Ray ni Tsh 408,564,000/= ikiwa haina UPS na katika gharama hizo inahusisha.

- Kufikisha na kusimika eneo husika
- Matengenezo ya miaka mitano (Comprehensive)
- Mafunzo kwa wataalam na watumiaji
- Upatikanaji wa wataalamu huduma inapokwama pamoja na vifaa kwa muda mfupi.

Wajumbe wa kikao waliomba kupunguziwa gharama kwa mzabuni na kutaka kupata ufafanuzi kwa nini gharama hizo hazihusishi UPS.

Mzabuni alieleza kuwa katika mashine inatakiwa kutumika kifaa kimoja cha umeme kama ni stabilizer/UPS pia kabla ya kufunga vifaa tiba hivyo ni lazima ufanyike upimaji wa umeme kuondoa hitilafu.

				Agreed price after	
_	ITEM	Supplier	Unit price	Negotiotion	Department
	ANAESTHETIC MACHINE	Anudha	51,840,000	51,000,000	EMD
_	Burr hole set	Anudha	1,500,000	1,470,000	EMD .
_	BLOOD GAS ANALYSER	Anudha	12,000,000	11,700,000	EMD
4	Video laryngoscope	Anudha	6,250,000	6,000,000	EMD
	Emergency curt	Anudha	1,500,000	1,750,000	EMD
$\overline{}$	Opthalmoscope	Anudha	1,400,000		EMD
	WALL MOUNTED OTOSCOPE	Anudha	1,400,000		EMD
	Pulse oximetry	Anudha	850,000	800,000	EMD
9	POP cast remover Electrical	Anudha	850,000	833,000	EMD
10	Suction device: powered (electric or pneumatic)	Anudha	1,350,000	1,300,000	EMD
11	Ward screens	Anudha	400,000	380,000	EMD
12	DIGITAL MOBILE XRAY	GE/COMPUTECH	280,316,470	275,316,470	EMD
	Diathermy machine	Kas Medics	16,000,000	15,520,000	EMD
	Ultrasound machine with	V AAI'	C4 000 000	62,720,000	EMD
	abdominal.linear and cardiac probe	Kas Medics	64,000,000		EMD
	OPERATING LAMP	Kas Medics	20,000,000	19,500,000	EMD
$\overline{}$	FOETAL MONITOR	Kas Medics	3,400,000	3,230,000	EMD
17	Automated external defibrilator	Kas Medics	3,500,000	3,395,000	EIVID
		- 11	11.11	Acused suiza a	Donortmont
	ITEM	Supplier	Unit price	Agreed price a	Department
	Continous or bi-level positive airway	-			
_1	pressure machine (CPAP, BiPAP)	Anudha	12,500,000	12,250,000	ICU
2	Phototherapy machine	Anudha	3,500,000	3,200,000	ICU
3	Infant baby warmer	Anudha	4,500,000	4,300,000	ICU
4	Defibrilator MACHINE with pacing capabilities	Anudha	23,900,000	26,400,000	tCU
	ECG machine with 12 lead electrodes	Anudha	5,200,000	5,000,000	ICU
	Heavy oxygen concentrator	Anudha	4,000,000	3,800,000	ICU
	Patient slide for stretcher transfers	Anudha	1,100,000	1,000,000	ICU
	PORTABLE ULTRASOUND MACHINE	Anudha	22,800,000	22,000,000	ICU
	Portable pt Cardiac Monitor	GE/COMPUTECH	21,060,000	19,560,000	ICU
	ICU Beds with CPR capability	Kas Medics	6,750,000	6,547,500	ICU
	Fluid warmer	Kas Medics	5,000,000	4,800,000	ICU
	Stretchers and gurneys (wheeled				
12	stretchers)	Kas Medics	2,500,000	2,400,000	ICU
_	Heavy suction machine	Kas Medics	2,800,000	2,730,000	ICU
_	Voltage stabiliser	Kas Medics	1,500,000	1,450,000	ICU
	INFUSION PUMP	Kas Medics	1,900,000	1,748,000	
_	SYRINGE PUMP	Kas Medics	2,009,000	1,840,000	icu
_	Laryngoscope with stylet and boudge	Kas Medics	1,800,000	1,800,000	ICU
_	Heavy duty mechanical ventirator	Mokasi	43,000,000	42,000,000	ICU
		Mokasi	18,000,000	17,550,000	ICU
19	I-start Machine	IMOKASI	10,000,000	17,000,000	1.30

A